

*TB 9-6625-2282-35

DEPARTMENT OF THE ARMY TECHNICAL BULLETIN

CALIBRATION PROCEDURE FOR TEST SET, ELECTRONIC SYSTEMS TS-4348/UV

Headquarters, Department of the Army, Washington, DC
9 August 2005

Distribution Statement A: Approved for public release; distribution is unlimited.

REPORTING OF ERRORS AND RECOMMENDING IMPROVEMENTS

You can improve this manual. If you find any mistakes or if you know of a way to improve these procedures, please let us know. Mail your letter or DA Form 2028 (Recommended Changes to Publications and Blank Forms) directly to Commander, US Army Aviation and Missile Command, AMSAM-MMC-MA-NP, Redstone Arsenal, AL 35898-5000. A reply will be furnished to you. You may also provide DA Form 2028 information to AMCOM via e-mail, fax, or the World Wide Web. Our FAX number is: DSN 788-6546 or Commercial 256-842-6546. Our e-mail address is: 2028@redstone.army.mil. Instructions for sending an electronic 2028 may be found at the back of this manual. For the World Wide Web, use: <https://amcom2028.redstone.army.mil>.

SECTION		Paragraph	Page
I.	IDENTIFICATION AND DESCRIPTION		
	Test instrument identification.....	1	2
	Forms, records, and reports	2	2
	Calibration description.....	3	2
II.	EQUIPMENT REQUIRMENTS		
	Equipment required	4	2
	Accessories required	5	3
III.	CALIBRATION PROCESS		
	Preliminary instructions	6	3
	Equipment setup	7	3
	Light level accuracy.....	8	4
	Final procedure.....	9	5

*This bulletin supersedes TB 9-6625-2282-35, dated 29 July 2002.

**SECTION I
IDENTIFICATION AND DESCRIPTION**

1. Test Instrument Identification. This bulletin provides instructions for the calibration of Test Set, Electronic Systems, TS-4348/UV. TM 11-5855-299-12&P was used as the prime data source in compiling these instructions. The equipment being calibrated will be referred to as the TI (test instrument) throughout this bulletin.

a. Model Variations. Variations among models are described in text.

b. Time and Technique. The time required for this calibration is approximately 1 hour, using the dc and low frequency technique.

2. Forms, Records, and Reports

a. Forms, records, and reports required for calibration personnel at all levels are prescribed by TB 750-25.

b. Adjustments to be reported are designated (R) at the end of a sentence in which they appear. Report only those adjustments made and designated with (R).

3. Calibration Description. TI parameters and performance specifications which pertain to this calibration are listed in table 1.

Table 1. Calibration Description

Test instrument parameters	Performance specifications ^{1, 2}
High light:	
GEN II	3.03×10^{-8} w/sr $\pm 50\%$
GEN III	1.43×10^{-8} w/sr $\pm 50\%$
Low light:	
GEN II	1.25×10^{-10} w/sr $\pm 32\%$
GEN III	5.55×10^{-11} w/sr $\pm 32\%$

¹Intensity levels reduced by 4% to account for reticle obscuration.

²Intensity level at 810 nm.

**SECTION II
EQUIPMENT REQUIREMENTS**

4. Equipment Required. Table 2 identifies the specific equipment to be used in this calibration procedure. This equipment is issued with Secondary Transfer Calibration Standards Set, AN/GSM-286. Alternate items may be used by the calibrating activity. The items selected must be verified to perform satisfactorily prior to use and must bear evidence of current calibration. The equipment must meet or exceed the minimum use specifications listed in table 2. The accuracies listed in table 2 provide a four-to-one ratio between the standard and TI.

5. Accessories Required. The accessories required for the calibration are common usage accessories, issued as indicated in paragraph 4 above and are not listed in this calibration procedure.

Table 2. Minimum Specifications of Equipment Required

Common name	Minimum use specifications	Manufacturer and model (part number)
NIGHT VISION DEVICE DETECTOR STANDARD	Wavelength range: 305 to 1000 nm Wavelength peak response: 720 nm ± 50 Responsitivity: 1.51×10^7 V/W sr ⁻¹ at 810 nm $\pm 8\%$ ($\pm 11\%$) Dynamic range: 6.6×10^{-13} to 4.6×10^{-7} Gain (elect): 10^9 V/A	(13335470)
MULTIMETER	Range: 0.62 to 732 mV Resolution: .01 mV Accuracy: $\pm 1.6\%$	Hewlett Packard, Model 3458A (3458A)

SECTION III CALIBRATION PROCESS

6. Preliminary Instructions

a. The instructions outlined in paragraphs 6 and 7 are preparatory to the calibration process. Personnel should become familiar with the entire bulletin before beginning the calibration.

b. Items of equipment used in this procedure are referenced within the text by common name as listed in table 2.

c. Unless otherwise specified, verify the result of each test and, whenever the test requirement is not met, take corrective action before continuing with the calibration. Adjustments required to calibrate the TI are included in this procedure. Additional maintenance information is contained in TM 11-5855-299-12&P.

d. Unless otherwise specified, all controls and control settings refer to the TI.

7. Equipment Setup

WARNING

HIGH VOLTAGE is used or exposed during the performance of this calibration. DEATH ON CONTACT may result if personnel fail to observe safety precautions. REDUCE OUTPUT(S) to minimum after each step within the performance check where applicable.

- a. Remove TI from protective case.
- b. Ensure TI II, III, OFF switch is set to OFF position.
- c. Set multimeter to measure dc volts and auto-ranging.

8. Light Level Accuracy

NOTE

If the night vision device detector standard is exposed to overload light conditions, several minutes are needed in low light level conditions for the night vision device detector standard to recover.

a. Performance Check

(1) Connect multimeter **INPUT HI** and **LO** to night vision device detector standard **BNC CONNECTOR** (fig. 2.)

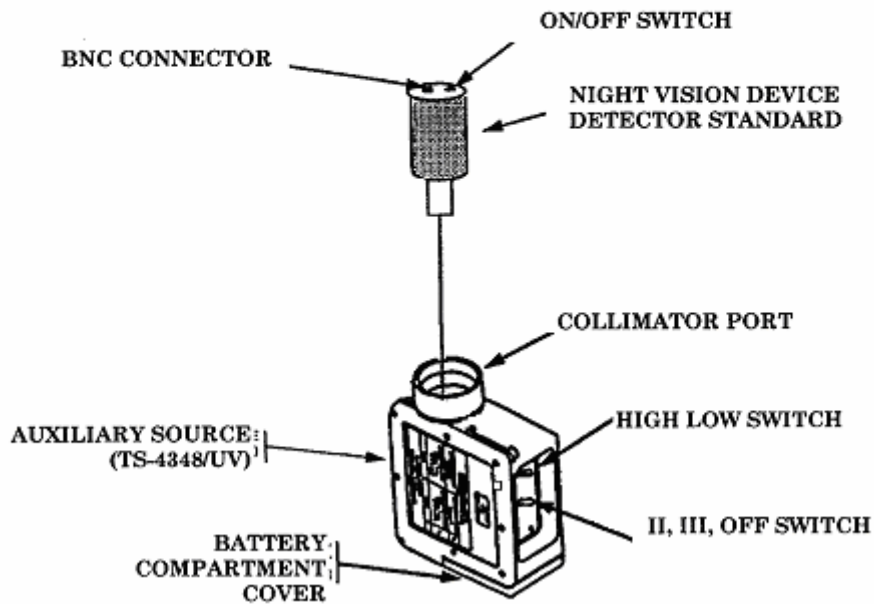


Figure 2. TS-4348/UV controls.

(2) Install night vision device detector standard into TI COLLIMATOR PORT (fig. 2).

(3) Turn night vision device detector standard power ON/OFF SWITCH (fig. 2) to ON and allow night vision detector standard to warm-up 15 minutes.

(4) Set TI **II, III, OFF** switch to **II**. Power indicator will illuminate.

NOTE

The night vision detector standard must always be rotated in the clockwise direction to prevent unscrewing the lens. Rotate the night vision detector standard a few degrees at a time then remove hand to allow reading to stabilize. Continue until maximum indication is obtained.

(5) Set TI **HIGH LOW** switch to **HIGH** and rotate night vision detector standard in TI collimator port to obtain peak output voltage. Multimeter will indicate between 229 and 686 mV dc.

(6) Set **II, III, OFF** switch to **III**. Multimeter will indicate between 108 and 323 mV dc.

(7) Set **HIGH LOW** switch to **LOW**.

(8) Set **II, III, OFF** switch to **OFF**. Wait at least 15 seconds and record multimeter indication.

(9) Set **II, III, OFF** switch to **II**. Multimeter will indicate between 1.28 and 2.49 mV dc after algebraically subtracting indication recorded in (8) above.

(10) Set **II, III, OFF** switch to **III**. Multimeter will indicate between .57 and 1.11 mV dc after algebraically subtracting indication recorded in (8) above.

(11) Set **II, III, OFF** switch to **OFF**.


b. Adjustments. No adjustments can be made.

9. Final Procedure

- a. Deenergize and disconnect all equipment and reinstall protective cover on TI.
- b. Annotate and affix DA label/form in accordance with TB 750-25.

By Order of the Secretary of the Army:

Official


SANDRA R. RILEY
*Administrative Assistant to the
Secretary of the Army*

0516006

PETER J. SCHOOMAKER
*General, United States Army
Chief of Staff*

Distribution:

To be distributed in accordance with the initial distribution number (IDN) 343398,
requirements for calibration procedure TB 9-6625-2282-35.

Instructions for Submitting an Electronic 2028

The following format must be used if submitting an electronic 2028. The subject line must be exactly the same and all fields must be included; however, only the following fields are mandatory: 1, 3, 4, 5, 6, 7, 8, 9, 10, 13, 15, 16, 17, and 27.

From: "Whomever" whomever@redstone.army.mil
To: <2028@redstone.army.mil

Subject: DA Form 2028

1. **From:** Joe Smith
2. **Unit:** home
3. **Address:** 4300 Park
4. **City:** Hometown
5. **St:** MO
6. **Zip:** 77777
7. **Date Sent:** 19-OCT -93
8. **Pub no:** 55-2840-229-23
9. **Pub Title:** TM
10. **Publication Date:** 04-JUL-85
11. **Change Number:** 7
12. **Submitter Rank:** MSG
13. **Submitter FName:** Joe
14. **Submitter MName:** T
15. **Submitter LName:** Smith
16. **Submitter Phone:** 123-123-1234
17. **Problem:** 1
18. **Page:** 2
19. **Paragraph:** 3
20. **Line:** 4
21. **NSN:** 5
22. **Reference:** 6
23. **Figure:** 7
24. **Table:** 8
25. **Item:** 9
26. **Total:** 123
27. **Text**

This is the text for the problem below line 27.

