

SCXI-1121

User Manual

Four-Channel Isolated Universal Transducer Module for Signal Conditioning

August 1994 Edition

Part Number 320426B-01

**© Copyright 1992, 1994 National Instruments Corporation.
All Rights Reserved.**

National Instruments Corporate Headquarters

6504 Bridge Point Parkway

Austin, TX 78730-5039

(512) 794-0100

Technical support fax: (800) 328-2203

(512) 794-5678

Branch Offices:

Australia (03) 879 9422, Austria (0662) 435986, Belgium 02/757.00.20, Canada (Ontario) (519) 622-9310,

Canada (Québec) (514) 694-8521, Denmark 45 76 26 00, Finland (90) 527 2321, France (1) 48 14 24 24,

Germany 089/741 31 30, Italy 02/48301892, Japan (03) 3788-1921, Netherlands 03480-33466, Norway 32-848400,

Spain (91) 640 0085, Sweden 08-730 49 70, Switzerland 056/20 51 51, U.K. 0635 523545

Limited Warranty

The SCXI-1121 is warranted against defects in materials and workmanship for a period of one year from the date of shipment, as evidenced by receipts or other documentation. National Instruments will, at its option, repair or replace equipment that proves to be defective during the warranty period. This warranty includes parts and labor.

A Return Material Authorization (RMA) number must be obtained from the factory and clearly marked on the outside of the package before any equipment will be accepted for warranty work. National Instruments will pay the shipping costs of returning to the owner parts which are covered by warranty.

National Instruments believes that the information in this manual is accurate. The document has been carefully reviewed for technical accuracy. In the event that technical or typographical errors exist, National Instruments reserves the right to make changes to subsequent editions of this document without prior notice to holders of this edition. The reader should consult National Instruments if errors are suspected. In no event shall National Instruments be liable for any damages arising out of or related to this document or the information contained in it.

EXCEPT AS SPECIFIED HEREIN, NATIONAL INSTRUMENTS MAKES NO WARRANTIES, EXPRESS OR IMPLIED, AND SPECIFICALLY DISCLAIMS ANY WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. CUSTOMER'S RIGHT TO RECOVER DAMAGES CAUSED BY FAULT OR NEGLIGENCE ON THE PART OF NATIONAL INSTRUMENTS SHALL BE LIMITED TO THE AMOUNT THEREFORE PAID BY THE CUSTOMER. NATIONAL INSTRUMENTS WILL NOT BE LIABLE FOR DAMAGES RESULTING FROM LOSS OF DATA, PROFITS, USE OF PRODUCTS, OR INCIDENTAL OR CONSEQUENTIAL DAMAGES, EVEN IF ADVISED OF THE POSSIBILITY THEREOF. This limitation of the liability of National Instruments will apply regardless of the form of action, whether in contract or tort, including negligence. Any action against National Instruments must be brought within one year after the cause of action accrues. National Instruments shall not be liable for any delay in performance due to causes beyond its reasonable control. The warranty provided herein does not cover damages, defects, malfunctions, or service failures caused by owner's failure to follow the National Instruments installation, operation, or maintenance instructions; owner's modification of the product; owner's abuse, misuse, or negligent acts; and power failure or surges, fire, flood, accident, actions of third parties, or other events outside reasonable control.

Copyright

Under the copyright laws, this publication may not be reproduced or transmitted in any form, electronic or mechanical, including photocopying, recording, storing in an information retrieval system, or translating, in whole or in part, without the prior written consent of National Instruments Corporation.

Trademarks

LabVIEW[®], NI-DAQ[®], and RTSI[®] are trademarks of National Instruments Corporation.

Product and company names listed are trademarks or trade names of their respective companies.

Warning Regarding Medical and Clinical Use of National Instruments Products

National Instruments products are not designed with components and testing intended to ensure a level of reliability suitable for use in treatment and diagnosis of humans. Applications of National Instruments products involving medical or clinical treatment can create a potential for accidental injury caused by product failure, or by errors on the part of the user or application designer. Any use or application of National Instruments products for or involving medical or clinical treatment must be performed by properly trained and qualified medical personnel, and all traditional medical safeguards, equipment, and procedures that are appropriate in the particular situation to prevent serious injury or death should always continue to be used when National Instruments products are being used. National Instruments products are NOT intended to be a substitute for any form of established process, procedure, or equipment used to monitor or safeguard human health and safety in medical or clinical treatment.

Contents

About This Manual

Organization of This Manual	xi
Conventions Used in This Manual	xii
Related Documentation	xiii
Customer Communication	xiii

Chapter 1

Introduction	1-1
What Your Kit Should Contain	1-1
Optional Software	1-2
Optional Equipment	1-3
Custom Cables	1-3
Unpacking	1-4

Chapter 2

Configuration and Installation	2-1
Module Configuration	2-1
Digital Signal Connections	2-4
Jumper W44	2-5
Jumper W38	2-5
Jumper W32	2-5
Using Jumpers W32 and W38	2-5
Analog Configuration	2-7
Grounding, Shielding, and Reference Mode Selection	2-7
Jumper W33	2-7
Input Channel Jumpers	2-8
Gain Jumpers	2-8
Filter Jumpers	2-9
Excitation Jumpers	2-10
Current and Voltage Excitation Jumpers	2-10
Excitation Level	2-10
Using the Internal Half-Bridge Completion	2-11
Hardware Installation	2-12
Signal Connections	2-13
Front Connector	2-13
Front Connector Signal Descriptions	2-15
Analog Input Channels	2-17
Excitation Channels	2-19
Temperature Sensor Connection	2-19
Connector-and-Shell Assembly	2-19
SCXI-1320, SCXI-1328, and SCXI-1321 Terminal Blocks	2-21
SCXI-1320 and SCXI-1328 Terminal Blocks	2-21
SCXI-1321 Offset-Null and Shunt-Calibration Terminal Block	2-21
SCXI-1321 Nulling Circuitry	2-21
Using the SCXI-1321 with RTDs and Thermistors	2-23
SCXI-1321 Shunt Calibration	2-24
Terminal Block Temperature Sensor	2-26
Terminal Block Jumper Configuration	2-27

Terminal Block Signal Connection	2-28
Terminal Block Installation	2-32
Rear Signal Connector	2-32
Rear Signal Connector Signal Descriptions	2-34
Analog Output Signal Connections	2-35
Digital I/O Signal Connections	2-35
Timing Requirements and Communication Protocol	2-37
Timing Signal	2-37
Communication Signals	2-37

Chapter 3

Theory of Operation	3-1
Functional Overview	3-1
SCXIbus Connector	3-2
SCXIbus Connector Signal Descriptions	3-4
Digital Interface	3-6
Digital Control Circuitry	3-7
Analog and Timing Circuitry	3-8
Analog Input Channels	3-8
Excitation Output Channels	3-10
Calibration	3-11
Calibration Equipment Requirements	3-11
Offset Null Adjust	3-12
Excitation Adjust	3-12
Analog Output Circuitry	3-14
Scanning Modes	3-15
Single-Module Parallel Scanning	3-15
Multiplexed Scanning	3-16
Single-Module Multiplexed Scanning	3-16
Single-Module Multiplexed Scanning (Direct)	3-16
Single-Module Multiplexed Scanning (Indirect)	3-17
Multiple-Module Multiplexed Scanning	3-17
Multiple-Chassis Scanning	3-18

Chapter 4

Register Descriptions	4-1
Register Description	4-1
Register Description Format	4-1
SCXI-1121 Registers	4-1
Module ID Register	4-2
Configuration Register	4-3
Slot 0 Register Descriptions	4-5
Slot-Select Register	4-6
Hardscan Control Register (HSCR)	4-7
FIFO Register	4-8

Chapter 5	
Programming	5-1
Programming Considerations	5-1
Notation	5-1
Register Writes	5-1
Register Selection and Write Procedure	5-2
Initialization	5-3
Single-Channel Measurements	5-3
Direct Measurements	5-3
Parallel Output	5-3
Multiplexed Output	5-3
Indirect Measurements	5-4
Measurements from Other Modules	5-4
Measurements from the SCXI-1121 via Another Module	5-5
Scanning Measurements	5-6
1. Data Acquisition Board Setup Programming	5-6
Counter 1 and SCANDIV	5-8
2. Module Programming	5-9
Single-Module Parallel Scanning	5-9
Single-Module Multiplexed Scanning (Direct)	5-9
Single-Module Multiplexed Scanning (Indirect)	5-9
Channel Scanning from Other Modules	5-9
Channel Scanning from the SCXI-1121 via Another	
Module	5-10
Multiple-Module Multiplexed Scanning	5-10
Multiple-Chassis Scanning	5-11
3. Programming the Slot 0 Hardscan Circuitry	5-11
4. Acquisition Enable, Triggering, and Servicing	5-12
Scanning Examples	5-13
Example 1	5-13
Example 2	5-13
Example 3	5-14
Appendix A	
Specifications	A-1
Analog Input	A-1
RTD Mode	A-2
Strain Gauge Mode	A-2
Cold-Junction Sensor	A-3
Physical	A-3
Operating Environment	A-4
Storage Environment	A-4
Appendix B	
Rear Signal Connector	B-1
Rear Signal Connector Signal Descriptions	B-2
Appendix C	
SCXIbus Connector	C-1
SCXIbus Connector Signal Descriptions	C-3
Appendix D	
SCXI-1121 Front Connector	D-1
Front Connector Signal Descriptions	D-2

Appendix E

SCXI-1121 Cabling	E-1
SCXI-1340 Cable Assembly	E-1
SCXI-1340 Installation	E-2
SCXI-1341 Lab-NB, Lab-PC, or Lab-PC+ and	
SCXI-1344 Lab-LC Cable Assembly	E-3
SCXI-1341 and SCXI-1344 Installation	E-4
SCXI-1342 PC-LPM-16 Cable Assembly	E-5
SCXI-1342 Installation	E-6
SCXI-1180 Feedthrough Panel	E-6
SCXI-1180 Installation	E-6
SCXI-1302 50-Pin Terminal Block	E-8
SCXI-1302 Wiring Procedure.....	E-8
SCXI-1302 Installation	E-9
SCXI-1351 One-Slot Cable Extender	E-9
SCXI-1351 Installation	E-10
SCXI-1350 Multichassis Adapter	E-10
SCXI-1350 Installation	E-10
SCXI-1343 Rear Screw Terminal Adapter	E-11
SCXI-1343 Installation	E-11

Appendix F

Revision A and B Photo and Parts Locator Diagrams	F-1
--	-----

Appendix G

Customer Communication	G-1
-------------------------------------	-----

Glossary	Glossary-1
-----------------------	------------

Index	Index-1
--------------------	---------

Figures

Figure 2-1.	SCXI-1121 General Parts Locator Diagram	2-2
Figure 2-2.	SCXI-1121 Detailed Parts Locator Diagram	2-3
Figure 2-3.	SCXI-1121 Front Connector Pin Assignment	2-14
Figure 2-4.	Ground-Referenced Signal Connection with High Common-Mode Voltage	2-17
Figure 2-5.	Floating Signal Connection Referenced to Chassis Ground for Better Signal-to-Noise Ratio	2-17
Figure 2-6.	Floating AC-Coupled Signal Connection	2-18
Figure 2-7.	AC-Coupled Signal Connection with High Common-Mode Voltage	2-18
Figure 2-8.	Assembling and Mounting the SCXI-1330 Connector-and-Shell Assembly	2-20
Figure 2-9.	Nulling Circuit	2-23
Figure 2-10.	Shunt Circuit	2-25
Figure 2-11.	SCXI-1320 Parts Locator Diagram	2-29
Figure 2-12.	SCXI-1328 Parts Locator Diagram	2-30
Figure 2-13.	SCXI-1321 Parts Locator Diagram	2-31
Figure 2-14.	SCXI-1121 Rear Signal Connector Pin Assignment	2-33
Figure 2-15.	SCANCLK Timing Requirements	2-37
Figure 2-16.	Slot-Select Timing Diagram	2-38
Figure 2-17.	Serial Data Timing Diagram	2-39
Figure 2-18.	Configuration Register Write Timing Diagram	2-40
Figure 2-19.	SCXI-1121 Module ID Register Timing Diagram	2-40
Figure 3-1.	SCXI-1121 Block Diagram	3-1
Figure 3-2.	SCXIbus Connector Pin Assignment	3-3
Figure 3-3.	Digital Interface Circuitry Block Diagram	3-6
Figure 3-4.	SCXI-1121 Digital Control	3-7
Figure 3-5.	Analog Input Block Diagram	3-9
Figure 3-6.	Analog Output Circuitry	3-14
Figure 3-7.	Single-Module Parallel Scanning	3-16
Figure 3-8.	Single-Module Multiplexed Scanning (Direct)	3-17
Figure 3-9.	Single-Module Multiplexed Scanning (Indirect)	3-17
Figure 3-10.	Multiple-Module Multiplexed Scanning	3-18
Figure 3-11.	Multiple-Chassis Scanning	3-18
Figure B-1.	SCXI-1121 Rear Signal Connector Pin Assignment	B-1
Figure C-1.	SCXIbus Connector Pin Assignment	C-2
Figure D-1.	SCXI-1121 Front Connector Pin Assignment	D-1
Figure E-1.	SCXI-1340 Installation	E-3
Figure E-2.	SCXI-1180 Rear Connections	E-7
Figure E-3.	SCXI-1180 Front Panel Installation	E-8
Figure E-4.	Cover Removal	E-9
Figure F-1.	Revision A and B SCXI-1121 Signal Conditioning Module	F-1
Figure F-2.	Revision A and B SCXI-1121 General Parts Locator Diagram	F-2
Figure F-3.	Revision A and B SCXI-1121 Detailed Parts Locator Diagram	F-3

Tables

Table 2-1.	Digital Signal Connections, Jumper Settings	2-6
Table 2-2.	Jumper W33 Settings	2-8
Table 2-3.	Gain Jumper Allocation	2-8
Table 2-4.	Gain Jumper Positions	2-9
Table 2-5.	Filter Jumper Allocation	2-9
Table 2-6.	Voltage and Current Mode Excitation Jumper Setup	2-10
Table 2-7.	Maximum Load per Excitation Channel	2-10
Table 2-8.	Excitation Level Jumper Selection	2-11
Table 2-9.	Completion Network Jumpers	2-12
Table 2-10.	Trimmer Potentiometer and Corresponding Channel	2-22
Table 2-11.	Nulling Resistors and Corresponding Channel	2-22
Table 2-12.	Jumper Settings of the Nulling Circuits	2-24
Table 2-13.	Jumper Settings on the SCXI-1320 Terminal Block	2-27
Table 2-14.	Jumper Settings on the SCXI-1328 Terminal Block	2-27
Table 2-15.	Jumper Settings on the SCXI-1321 Terminal Block	2-28
Table 2-16.	SCXIbus to SCXI-1121 Rear Signal Connector to Data Acquisition Board Pin Equivalences	2-36
Table 3-1.	SCXIbus Equivalents for the Rear Signal Connector	3-5
Table 3-2.	Calibration Potentiometer Reference Designators	3-13
Table 5-1.	SCXI-1121 Rear Signal Connector Pin Equivalences	5-2
Table E-1.	SCXI-1121 and MIO-16 Pinout Equivalences	E-2
Table E-2.	SCXI-1341 and SCXI-1344 Pin Translations	E-4
Table E-3.	SCXI-1342 Pin Translations	E-5
Table E-4.	SCXI-1343 Pin Connections	E-12

About This Manual

This manual describes the electrical and mechanical aspects of the SCXI-1121 and contains information concerning its operation and programming. The SCXI-1121 is a member of the National Instruments Signal Conditioning eXtensions for Instrumentation (SCXI) Series for the National Instruments data acquisition plug-in boards. This board is designed for signal conditioning of strain gauges, RTDs, thermistors, thermocouples, volt and millivolt sources, and 4 to 20 mA sources or 0 to 20 mA process-current sources where high common-mode voltages exist. The SCXI-1121 operates as four isolated input channels and four isolated excitation channels. Each channel is isolated and independently configurable via jumpers.

This manual describes the installation, basic programming considerations, and theory of operation for the SCXI-1121.

Organization of This Manual

The *SCXI-1121 User Manual* is organized as follows:

- Chapter 1, *Introduction*, describes the SCXI-1121; lists the contents of your SCXI-1121 kit; describes the optional software, optional equipment, and custom cables; and explains how to unpack the SCXI-1121 kit.
- Chapter 2, *Configuration and Installation*, describes the SCXI-1121 jumper configurations, installation of the SCXI-1121 into the SCXI chassis, signal connections to the SCXI-1121, and cable wiring.
- Chapter 3, *Theory of Operation*, contains a functional overview of the SCXI-1121 module and explains the operation of each functional unit making up the SCXI-1121.
- Chapter 4, *Register Descriptions*, describes in detail the SCXI-1121 Module ID Register, the Configuration Register, the Slot 0 registers, and multiplexer addressing.
- Chapter 5, *Programming*, contains a functional programming description of the SCXI-1121 and Slot 0.
- Appendix A, *Specifications*, lists the specifications for the SCXI-1121.
- Appendix B, *Rear Signal Connector*, describes the pinout and signal names for the SCXI-1121 50-pin rear signal connector, including a description of each connection.
- Appendix C, *SCXIBus Connector*, describes the pinout and signal names for the SCXI-1121 96-pin SCXIBus connector, including a description of each connection.
- Appendix D, *SCXI-1121 Front Connector*, describes the pinout and signal names for the SCXI-1121 front connector, including a description of each connection.
- Appendix E, *SCXI-1121 Cabling*, describes how to use and install the hardware accessories for the SCXI-1121.

- Appendix F, *Revision A and B Photo and Parts Locator Diagrams*, contains a photograph of the Revision A and B SCXI-1121 signal conditioning module and the general and detailed parts locator diagrams.
- Appendix G, *Customer Communication*, contains forms you can use to request help from National Instruments or to comment on our products.
- The *Glossary* contains an alphabetical list and description of terms used in this manual, including abbreviations, acronyms, metric prefixes, mnemonics, symbols, and terms.
- The *Index* contains an alphabetical list of key terms and topics in this manual, including the page where you can find each one.

Conventions Used in This Manual

The following conventions are used in this manual.

<i>italic</i>	Italic text denotes emphasis, a cross reference, or an introduction to a key concept.
Lab board	Lab board refers to the Lab-LC, Lab-NB, Lab-PC, and Lab-PC+ boards unless otherwise noted.
MC	MC refers to the Micro Channel series computers.
MIO board	MIO board refers to the National Instruments multichannel I/O data acquisition boards, AT-MIO-16, MC-MIO-16, AT-MIO-16F-5, AT-MIO-16X, AT-MIO-16D, AT-MIO-64F-5, NB-MIO-16, and NB-MIO-16X, unless otherwise noted.
monospace	Lowercase text in this font denotes text or characters that are to be literally input from the keyboard, sections of code, programming examples, and syntax examples. This font is also used for the proper names of disk drives, paths, directories, programs, subprograms, subroutines, device names, functions, variables, filenames, and extensions, and for statements and comments taken from program code.
NB	NB refers to the NuBus series computers.
PC	PC refers to the IBM PC/XT, the IBM PC AT, and compatible computers.
SCXIBus	SCXIBus refers to the backplane in the chassis. A signal on the backplane is referred to as the SCXIBus <signal name> line (or signal). The SCXIBus descriptor may be omitted when the meaning is clear. Descriptions of all SCXIBus signals are given in Appendix C, <i>SCXIBus Connector</i> .
Slot 0	Slot 0 refers to the power supply and control circuitry in the SCXI chassis.

Abbreviations, acronyms, metric prefixes, mnemonics, symbols, and terms are listed in the *Glossary*.

Related Documentation

The following documents contain information that you may find helpful as you read this manual:

- *AT-MIO-16 User Manual* (part number 320476-01)
- *AT-MIO-16D User Manual* (part number 320489-01)
- *AT-MIO-16F-5 User Manual* (part number 320266-01)
- *AT-MIO-16X User Manual* (part number 320488-01)
- *AT-MIO-64F-5 User Manual* (part number 320487-01)
- *Lab-LC User Manual* (part number 320380-01)
- *Lab-NB User Manual* (part number 320174-01)
- *Lab-PC User Manual* (part number 320205-01)
- *Lab-PC+ User Manual* (part number 320502-01)
- *MC-MIO-16 User Manual, Revisions A to C* (part number 320130-01)
- *MC-MIO-16 User Manual, Revision D* (part number 320560-01)
- *NB-MIO-16 User Manual* (part number 320295-01)
- *NB-MIO-16X User Manual* (part number 320157-01)
- *PC-LPM-16 User Manual* (part number 320287-01)
- *SCXI-1000/1001 User Manual* (part number 320423-01)

Customer Communication

National Instruments wants to receive your comments on our products and manuals. We are interested in the applications you develop with our products, and we want to help if you have problems with them. To make it easy for you to contact us, this manual contains comment and configuration forms for you to complete. These forms are in Appendix G, *Customer Communication*, at the end of this manual.

Chapter 1

Introduction

This chapter describes the SCXI-1121; lists the contents of your SCXI-1121 kit; describes the optional software, optional equipment, and custom cables; and explains how to unpack the SCXI-1121 kit.

The SCXI-1121 consists of four isolated input channels and four isolated excitation channels. The SCXI-1121 is a module for signal conditioning of strain gauges, RTDs, thermistors, thermocouples, volt and millivolt sources, 4 to 20 mA current sources, and 0 to 20 mA process-current sources. The SCXI-1121 can operate in two output modes—the Parallel-Output mode with all four input channels connected in parallel to four data acquisition board channels, or the Multiplexed-Output mode with all four channels multiplexed into a single data acquisition board channel.

The SCXI-1121 operates with full functionality with National Instruments MIO-16 boards. The SCXI-1121 operates with full functionality with the Lab-PC+ board in single-chassis SCXI systems. However, the Lab-PC+ cannot control multiple-chassis SCXI systems. You can use the Lab-NB, the Lab-PC, the Lab-LC, and the PC-LPM-16 boards with the SCXI-1121, but these boards can control only single-chassis SCXI systems and cannot scan the module when it is configured in the Multiplexed-Output mode. These boards can perform only single-channel reads in this mode. You can also use the SCXI-1121 with other systems that comply with the specifications given in Chapter 2, *Configuration and Installation*. You can multiplex several SCXI-1121s into a single channel, thus greatly increasing the number of analog input signals that can be digitized.

The addition of a shielded terminal block provides screw terminals for easy signal attachment to the SCXI-1121. In addition, a temperature sensor for cold-junction compensation of thermocouples is included on the terminal block. This cold-junction reference (CJR) is either multiplexed along with the four input channels or connected by jumpers to a different channel of the data acquisition board.

With the SCXI-1121, the SCXI chassis can serve as a fast-scanning signal conditioner for laboratory testing, production testing, and industrial process monitoring.

What Your Kit Should Contain

The contents of the SCXI-1121 kit (part number 776572-21) are listed as follows:

Kit Component	Part Number
SCXI-1121 module	181700-01
<i>SCXI-1121 User Manual</i>	320426-01

If your kit is missing any of the components, contact National Instruments.

Optional Software

This manual contains complete instructions for directly programming the SCXI-1121. You can order separate software packages for controlling the SCXI-1121 from National Instruments.

When you combine the PC, AT, and MC data acquisition boards with the SCXI-1121, you can use LabVIEW for Windows or LabWindows for DOS. LabVIEW and LabWindows are innovative program development software packages for data acquisition and control applications. LabVIEW uses graphical programming, whereas LabWindows enhances Microsoft C and QuickBASIC. Both packages include extensive libraries for data acquisition, instrument control, data analysis, and graphical data presentation.

Your National Instruments data acquisition board is shipped with the NI-DAQ software. NI-DAQ has a library of functions that you can call from your application programming environment. These functions include routines for analog input (A/D conversion), buffered data acquisition (high-speed A/D conversion), analog output (D/A conversion), waveform generation, digital I/O, counter/timer, SCXI, RTSI, and self-calibration. NI-DAQ maintains a consistent software interface among its different versions so you can switch between platforms with minimal modifications to your code.

You can also use the SCXI-1121, together with the PC, AT, and MC data acquisition boards, with NI-DAQ software for DOS/Windows/LabWindows. NI-DAQ software for DOS/Windows/LabWindows comes with language interfaces for Professional BASIC, Turbo Pascal, Turbo C, Turbo C++, Borland C++, and Microsoft C for DOS; and Visual Basic, Turbo Pascal, Microsoft C with SDK, and Borland C++ for Windows. NI-DAQ software for DOS/Windows/LabWindows is on high-density 5.25 in. and 3.5 in. diskettes.

You can use the SCXI-1121, together with the Lab-LC or NB Series data acquisition boards, with LabVIEW for Macintosh, a software system that features interactive graphics, a state-of-the-art user interface, and a powerful graphical programming language. The LabVIEW Data Acquisition VI Library, a series of VIs for using LabVIEW with National Instruments boards, is included with LabVIEW. The LabVIEW Data Acquisition VI Library is functionally equivalent to the NI-DAQ software for Macintosh.

You can also use the SCXI-1121, combined with the NB Series data acquisition boards, with NI-DAQ software for Macintosh. NI-DAQ software for Macintosh, which is shipped with all National Instruments Macintosh data acquisition boards, comes with language interfaces for MPW C, THINK C, Pascal, and Microsoft QuickBASIC. Any language that uses Device Manager Toolbox calls can access NI-DAQ software for Macintosh.

Optional Equipment

Equipment	Part Number
NB6 cable	
0.5 m	181305-01
1.0 m	181305-10
SCXI-1320 front terminal block	776573-20
SCXI-1321 offset-null and shunt-calibration terminal block	776573-21
SCXI-1328 high-accuracy isothermal terminal block	776573-28
SCXI-1330 32-pin connector-and-shell assembly	776573-30
SCXI-1340 cable assembly	776574-40
SCXI-1341 Lab-NB/Lab-PC/Lab-PC+ cable assembly	776574-41
SCXI-1342 PC-LPM-16 cable assembly	776574-42
SCXI-1343 rear screw terminal adapter	776574-43
SCXI-1344 Lab-LC cable assembly	776574-44
SCXI-1346 shielded multichassis cable adapter	776574-46
SCXI-1347 SCXI shielded cable assembly	
with 1 m cable	776574-471
with 2 m cable	776574-472
with 5 m cable	776574-475
with 10 m cable	776574-470
SCXI-1349 SCXI shielded cable assembly	
with 1 m cable	776574-491
with 2 m cable	776574-492
with 5 m cable	776574-495
with 10 m cable	776574-490
SCXI-1350 multichassis adapter	776575-50
SCXI process-current resistor kit	776582-01
Standard ribbon cable	
0.5 m	180524-05
1.0 m	180524-10

Refer to the *Signal Connections* section in Chapter 2, *Configuration and Installation*, and to Appendix E, *SCXI-1121 Cabling*, for additional information on cabling, connectors, and adapters.

Custom Cables

The SCXI-1121 rear signal connector is a 50-pin male ribbon-cable header. The manufacturer part number used by National Instruments for this header is as follows:

- AMP Inc. (part number 1-103310-0)

The mating connector for the SCXI-1121 rear signal connector is a 50-position polarized ribbon-socket connector with strain relief. National Instruments uses a polarized or keyed connector to prevent inadvertent upside-down connection to the SCXI-1121. Recommended manufacturer part numbers for this mating connector are as follows:

- Electronic Products Division/3M (part number 3425-7650)
- T&B/Ansley Corporation (part number 609-5041CE)

Standard 50-conductor, 28 AWG, stranded ribbon cables that can be used with these connectors are as follows:

- Electronic Products Division/3M (part number 3365/50)
- T&B/Ansley Corporation (part number 171-50)

The SCXI-1121 front connector is a 32-pin DIN C male connector with column A and column C even pins only. The manufacturer part number used by National Instruments for this connector is as follows:

- Panduit Corporation (part number 100-932-023)

The mating connector for the SCXI-1121 front connector is a 32-pin DIN C female connector. National Instruments uses a polarized connector to prevent inadvertent upside-down connection to the SCXI-1121. Recommended manufacturer part numbers for this mating connector are as follows:

- Panduit Corporation (part number 100-932-434; straight-solder eyelet pins)
- Panduit Corporation (part number 100-932-633; right-angle pins)

National Instruments selected these connectors to meet UL 1950 and UL 1244 for 1,500 Vrms isolation.

Unpacking

Your SCXI-1121 module is shipped in an antistatic package to prevent electrostatic damage to the module. Several components on the module can be damaged by electrostatic discharge. To avoid such damage in handling the module, take the following precautions.

- Touch the antistatic package to a metal part of your SCXI chassis before removing the module from the package.
- Remove the module from the package and inspect the module for loose components or any other sign of damage. Notify National Instruments if the module appears damaged in any way. *Do not* install a damaged module into your SCXI chassis.

Chapter 2

Configuration and Installation

This chapter describes the SCXI-1121 jumper configurations, installation of the SCXI-1121 into the SCXI chassis, signal connections to the SCXI-1121, and cable wiring.

Module Configuration

The SCXI-1121 contains 49 jumpers that are shown in the parts locator diagrams in Figures 2-1 and 2-2.




Figure 2-1. SCXI-1121 General Parts Locator Diagram




Figure 2-2. SCXI-1121 Detailed Parts Locator Diagram

The jumpers are used as follows:

- Fixed jumpers
 - On Revision A and B modules, jumper W32 is unused and should not be connected.
 - Jumper W45 is reserved and should not be reconfigured.
 - On Revision A and B modules, jumper W44 carries the SLOT0SEL* signal from the rear signal connector, after buffering, to the SCXIbus INTR* line and should be left in the factory-set position (position 1). On Revision C or later modules, jumper W44 does not exist.
- User-configurable jumpers
 - Jumper W38 carries the SCXIbus MISO line, after buffering, to the SERDATOUT signal on the rear signal connector.
 - On Revision C or later modules, jumper W32 connects a pullup resistor to the SERDATOUT signal on the rear signal connector.
 - Jumper W33 configures the guard, the analog output ground, and enables the Pseudodifferential Reference mode.
 - Jumpers W3, W19, W29, and W41 configure the first-stage gain of input channels 0 through 3, respectively.
 - Jumpers W4, W20, W30, and W42 configure the second-stage gain of input channels 0 through 3, respectively.
 - Jumpers W5, W21, W31, and W43 configure the first-stage filtering of input channels 0 through 3, respectively.
 - Jumpers W6 and W7, W8 and W9, W10 and W11, and W12 and W13 configure the second-stage filtering of input channels 0 through 3, respectively.
 - Jumpers W14 and W15, W22 and W23, W34 and W35, and W46 and W47 configure the voltage or current mode of operation for excitation channels 0 through 3, respectively.
 - Jumpers W16 and W26, W24 and W25, W36 and W37, and W48 and W49 configure the level of excitation for excitation channels 0 through 3, respectively.
 - Jumpers W1 and W2, W17 and W18, W27 and W28, and W39 and W40 configure the half-bridge completion network for channels 0 through 3, respectively.

Further configuration of the board is software controlled and will be discussed later in this chapter.

Digital Signal Connections

The SCXI-1121 has three jumpers dedicated for communication between the data acquisition board and the SCXIbus. These jumpers are W32, W38, and W44.

Jumper W44

Position 1 on Revision A and B modules connects, after buffering, SLOTOSEL* to the SCXIBus INTR* line. This is the factory-default setting and should not be changed. In this setting, the data acquisition board controls the SCXIBus INTR* line. See the *Timing Requirements and Communication Protocol* section later in this chapter, and Chapter 5, *Programming*, for information on the use of the INTR* line. See Appendix E, *SCXI-1121 Cabling*, for the pin equivalences of the SCXI-1121 rear signal connector and the data acquisition board I/O connector.

Position 3 is reserved and should not be used. This position is not explicitly marked on the module.

On Revision C or later modules, jumper W44 does not exist. SLOTOSEL* is always buffered to the INTR* line.

Jumper W38

Position 1 connects, after buffering, the SCXIBus MISO line to the SERDATOUT pin of the rear signal connector. In this setting, along with the proper setting of W32, the data acquisition board can read the Module ID Register of the SCXI-1121. See the *Timing Requirements and Communication Protocol* section later in this chapter, and Chapter 4, *Register Descriptions*, for information on reading the Module ID Register. See Appendix E, *SCXI-1121 Cabling*, for the pin equivalences of the SCXI-1121 rear signal connector and the data acquisition board I/O connector. This is the factory-default setting.

Position 3 disconnects SERDATOUT from the SCXIBus MISO line.

Jumper W32

On Revision A and B modules, jumper W32 should not be connected. On Revision C or later modules, Position 1 connects a 2.2 k Ω pullup resistor to the SERDATOUT line (factory-default setting), and Position 3 does not connect the pullup resistor to the SERDATOUT line.

Using Jumpers W32 and W38

Set jumpers W32 and W38 as follows:

If the SCXI-1121 is not cabled to a data acquisition board, the positions of these jumpers do not matter, so leave them in their factory default positions (both in position 1).

If the SCXI-1121 is cabled to a data acquisition board, and the SCXI chassis that the SCXI-1121 is in, is the only SCXI chassis cabled to that data acquisition board, leave the jumpers in their factory default positions (both in position 1).

If the SCXI-1121 is cabled to a data acquisition board, and there are multiple SCXI chassis cabled to that data acquisition board with shielded cables (you are using SCXI-1346 shielded cable multi-chassis adapters), leave the jumpers in their factory default positions (both in position 1).

If the SCXI-1121 is cabled to a data acquisition board, and there are multiple SCXI chassis cabled to that data acquisition board with ribbon cables (you are using SCXI-1350 multi-chassis adapters), leave jumper W38 in its factory default position (position 1). On all but one of the SCXI-1121s that are cabled to the data acquisition board, move jumper W32 to position 3. It does not matter which of the SCXI-1121 modules that are cabled to the data acquisition board has jumper W32 set to position 1. If you have different types of modules cabled to the data acquisition board, those different modules will have jumpers similar to W38 and W32 of the SCXI-1121. Set those jumpers on the different modules using the same method described here for the SCXI-1121.



On Revision A and B SCXI-1121s, jumper W32 is not used. You set jumper W38 as explained in the cases above, except in the case of a multiple chassis ribbon cable system. In a multichassis ribbon cable system with Revision A and B SCXI-1121s cabled to the data acquisition board, you can access the MISO line in only one chassis. Pick one of the chassis and set jumper W38 to position 1 on the SCXI-1121 in that chassis that is cabled to the data acquisition board. On the SCXI-1121s that are in the other chassis and cabled to the data acquisition board, set jumper W38 to position 3. Notice that you will only be able to access digital information from the chassis that has the SCXI-1121 with jumper W38 set to position 1.

Table 2-1. Digital Signal Connections, Jumper Settings

Jumper	Description	Configuration
W38	Factory setting; connects MISO to SERDATOUT	
W38	Parking position	
W45	Factory setting	
W44	Factory setting (Revision A and B modules only)	

(continues)

Table 2-1. Digital Signal Connections, Jumper Settings (Continued)

Jumper	Description	Configuration
W32	Factory-default setting; connects pullup to SERDATOUT (Revision C and later)	
W32	Parking position (not connected on Revision A or B modules)	

Analog Configuration

The SCXI-1121 has 45 analog configuration jumpers.

Before starting, notice that the jumper configurations for each input channel and each excitation channel are similar; only the jumper numbers differ. Therefore, when you learn how to set up one channel pair (input and excitation), you can set up the other channel pairs as well.

Grounding, Shielding, and Reference Mode Selection

Jumper W33

Position AB-R0 connects the analog reference to the analog output ground (pins 1 and 2 on the rear signal connector). Select this configuration if you are using an RSE data acquisition board. It is not recommended to use a differential input data acquisition board when jumper W33 is in the AB-R0 position.

Position AB-R1 connects the analog reference to the SCXibus guard.

Position A-R0R1 is the parking position and the factory setting.

Position AB-R2 enables the Pseudodifferential Reference mode and connects the analog reference to the OUTREF pin on the rear signal connector. Select this mode when the SCXI-1121 has to operate with data acquisition boards that have a nonreferenced single-ended (NRSE) input. It is not recommended to use differential-input data acquisition boards when jumper W33 is in the AB-R2 position.

Table 2-2. Jumper W33 Settings

Jumper	Description	Configuration
W33	Factory setting in parking position	<p>A 2x3 grid representing jumper settings. The columns are labeled R2, R1, and R0. The rows are labeled A and B. In the factory setting, the top-right cell (R0, A) is shaded black, and the bottom-left cell (R2, B) is shaded black. All other cells are white with a dot in the center.</p>
W33	Connects the analog reference to AOGND (pins 1 and 2 of the rear signal connector)	<p>A 2x3 grid representing jumper settings. The columns are labeled R2, R1, and R0. The rows are labeled A and B. In this configuration, the top-right cell (R0, A) is shaded black, and the bottom-left cell (R2, B) is shaded black. All other cells are white with a dot in the center.</p>
W33	Connects SCXIbus guard to the analog reference	<p>A 2x3 grid representing jumper settings. The columns are labeled R2, R1, and R0. The rows are labeled A and B. In this configuration, the top-left cell (R2, A) is shaded black, the top-right cell (R0, A) is shaded black, and the bottom-middle cell (R1, B) is shaded black. All other cells are white with a dot in the center.</p>
W33	Enables the Pseudodifferential Reference mode (pin 19 of the rear signal connector is connected to the analog reference)	<p>A 2x3 grid representing jumper settings. The columns are labeled R2, R1, and R0. The rows are labeled A and B. In this configuration, the top-left cell (R2, A) is shaded black, and the bottom-left cell (R2, B) is shaded black. All other cells are white with a dot in the center.</p>

Input Channel Jumpers

Gain Jumpers

Each input channel has two gain stages. The first gain stage provides gains of 1, 10, 50, and 100 and the second stage provides gains of 1, 2, 5, 10, and 20. Tables 2-3 and 2-4 show how to set up the gain for each channel.

Table 2-3. Gain Jumper Allocation

Input Channel Number	First Gain Jumper	Second Gain Jumper
0	W3	W4
1	W19	W20
2	W29	W30
3	W41	W42

The board is shipped to you with the first-stage gain set to 100 (position A) and a second-stage gain set to 10 (position D). To change the gain of your module, move the appropriate jumper on your module to the position indicated in Table 2-4. Refer to Figure 2-2 for the jumper locations on your module.

To determine the overall gain of a given channel use the following formula:

$$\text{Overall gain} = \text{First-stage gain} \times \text{second-stage gain.}$$

Table 2-4. Gain Jumper Positions

Gain	Setting	Jumper Position
First-stage	1	D
	10	C
	50	B
	100	A (factory setting)
Second-stage	1	A
	2	B
	5	C
	10	D (factory setting)
	20	E

Filter Jumpers

Two-stage filtering is also available on your SCXI-1121 module. The first stage is located in the isolated section of the input channel, whereas the second stage is located in the nonisolated section of the input channel. This permits a higher signal-to-noise ratio by eliminating the noise generated by the isolation amplifier. Furthermore, two filter bandwidths are available—10 kHz and 4 Hz.

Table 2-5. Filter Jumper Allocation

Input Channel Number	First Filter Jumper		Second Filter Jumper	
	4 Hz (Factory Setting)	10 kHz	4 Hz (Factory Setting)	10 kHz
0	W5-A	W5-B	W6	W7
1	W21-A	W21-B	W8	W9
2	W31-A	W31-B	W10	W11
3	W43-A	W43-B	W12	W13

Your SCXI-1121 is shipped in the 4 Hz configuration. Always make sure to set both stages to the same bandwidth. This will ensure that the required bandwidth is achieved.

Excitation Jumpers

Current and Voltage Excitation Jumpers

You can configure each excitation channel of your SCXI-1121 to either a Voltage or Current excitation mode. Each channel has two jumpers for this purpose. Set both jumpers in the same mode for correct operation of the excitation channel. Refer to Table 2-6 for setting up your module in the mode you want. Your SCXI-1121 is shipped to you in the Voltage mode.

Table 2-6. Voltage and Current Mode Excitation Jumper Setup

Excitation Channel	Jumpers	Voltage Mode (Factory Setting)	Current Mode
0	W14 and W15		
1	W22 and W23		
2	W34 and W35		
3	W46 and W47		

Excitation Level

Each excitation channel of your SCXI-1121 has two different current or voltage levels. You can set a given channel to one of the following level modes:

- In the Current mode – 0.150 or 0.450 mA
- In the Voltage mode – 3.333 or 10 V

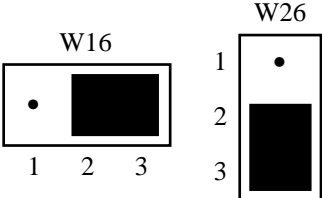
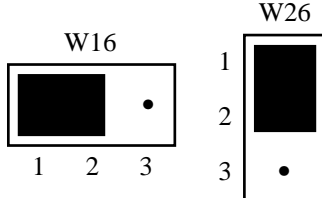






It is important to notice that you should select the level of excitation according to the load you are using. Table 2-7 lists the maximum load that can be driven per channel at each level of excitation for both volt and current excitation.

Table 2-7. Maximum Load per Excitation Channel

Excitation Level	Maximum Load
3.333 V	28 mA
10 V	14 mA
0.150 mA	10 kΩ
0.450 mA	10 kΩ

After selecting the excitation mode of operation desired—Voltage or Current—as described in the previous section, use Table 2-8 to set your SCXI-1121 for the level of operation. Your SCXI-1121 is shipped with the Voltage mode set to 3.333 V.

Table 2-8. Excitation Level Jumper Selection

Excitation Channel	Jumpers	3.333 V or 0.150 mA (Factory Setting)	10 V or 0.450 mA
0	W16 and W26		
1	W24 and W25		
2	W36 and W37		
3	W48 and W49		

















Using the Internal Half-Bridge Completion

Your SCXI-1121 includes half-bridge completion for half-bridge and quarter-bridge setups. The completion network consists of two $4.5 \text{ k}\Omega \pm 0.05\%$ ratio tolerance resistors with a temperature coefficient of $5 \text{ ppm}/^\circ\text{C}$. These resistors are connected in series. To enable the network, you must set two jumpers for each input/excitation channel pair.

When the completion network is enabled, you cannot access the negative input of the amplifier, which preserves the overvoltage protection of the channel. Table 2-9 shows how to enable and disable the completion network.

Note: *When using the half-bridge completion network with a quarter-bridge setup, you must use an extra resistor to complete the bridge. Place this resistor on the terminal block between the positive input channel and the negative excitation output.*

Table 2-9. Completion Network Jumpers

Channel	Jumpers	Enable Completion	Disable Network (Factory Setting)
0	W1 and W2	 W2 A B  W1 1 2 3	 W2 A B  W1 1 2 3
1	W17 and W18	 W18 A B  W17 1 2 3	 W18 A B  W17 1 2 3
2	W27 and W28	 W28 A B  W27 1 2 3	 W28 A B  W27 1 2 3
3	W39 and W40	 W40 A B  W39 1 2 3	 W40 A B  W39 1 2 3

Hardware Installation

You can install the SCXI-1121 in any available SCXI chassis. After you have made any necessary changes and have verified and recorded the jumper settings on the form in Appendix G, *Customer Communication*, you are ready to install the SCXI-1121. The following are general installation instructions; consult the user manual or technical reference manual of your SCXI chassis for specific instructions and warnings.

1. Turn off the computer that contains the data acquisition board or disconnect it from your SCXI chassis.
2. Turn off the SCXI chassis. Do not insert the SCXI-1121 into a chassis that is turned on.
3. Insert the SCXI-1121 into the board guides. Gently guide the module into the back of the slot until the connectors make good contact. If a cable assembly has already been installed in the rear of the chassis, the module and cable assembly must be firmly engaged; however, do not *force* the module into place.
4. Screw the front mounting panel of the SCXI-1121 to the top and bottom threaded strips of your SCXI chassis.
5. If this module is to be connected to an MIO-16 data acquisition board, attach the connector at the metal end of the SCXI-1340 cable assembly to the rear signal connector on the SCXI-1121 module. Screw the rear panel to the rear threaded strip. Attach the loose end of the cable to the MIO-16 board.

Note: For installation procedures with other SCXI accessories and data acquisition boards, consult Appendix E, *SCXI-1121 Cabling*.

6. Check the installation.
7. Turn on the SCXI chassis.
8. Turn on the computer or reconnect it to your chassis.

The SCXI-1121 module is installed and ready for operation.

Signal Connections

This section describes the input and output signal connections to the SCXI-1121 board via the SCXI-1121 front connector and rear signal connector, and includes specifications and connection instructions for the signals given on the SCXI-1121 connectors.

Warning: *Connections that exceed any of the maximum ratings of input or output signals on the SCXI-1121 can result in damage to the SCXI-1121 module and to the SCXIbus. Maximum input ratings for each signal are given in this chapter under the discussion of that signal. National Instruments is NOT liable for any damages resulting from such signal connections.*

Front Connector

Figure 2-3 shows the pin assignments for the SCXI-1121 front connector.

Pin Number	Signal Name	Column			Signal Name
		A	B	C	
32	CH0+	○	○	○	CH0-
31		○	○	○	
30	EX0+	○	○	○	EX0+
29		○	○	○	
28	EGND0	○	○	○	
27		○	○	○	
26	CH1+	○	○	○	CH1-
25		○	○	○	
24	EX1+	○	○	○	EX1-
23		○	○	○	
22	EGND1	○	○	○	
21		○	○	○	
20	CH2+	○	○	○	CH2-
19		○	○	○	
18	EX2+	○	○	○	EX2-
17		○	○	○	
16	EGND2	○	○	○	
15		○	○	○	
14	CH3+	○	○	○	CH3-
13		○	○	○	
12	EX3+	○	○	○	EX3-
11		○	○	○	
10	EGND3	○	○	○	
9		○	○	○	
8		○	○	○	RSVD
7		○	○	○	
6	SCAL	○	○	○	RSVD
5		○	○	○	
4	+5 V	○	○	○	MTEMP
3		○	○	○	
2	CGND	○	○	○	DTEMP
1		○	○	○	

Figure 2-3. SCXI-1121 Front Connector Pin Assignment

Front Connector Signal Descriptions

Pin	Signal Name	Description
A2	CGND	Chassis Ground – This pin is tied to the SCXI chassis.
C2	DTEMP	Direct Temperature Sensor – This pin connects the temperature sensor to the MCH4+ when the terminal block is configured for direct temperature connection.
A4	+5 V	+5 VDC Source – This pin is used to power the temperature sensor on the terminal block. 0.2 mA of source not protected.
C4	MTEMP	Multiplexed Temperature Sensor – This pin connects the temperature sensor to the output multiplexer.
A6	SCAL	Shunt Calibration – This pin is tied to the SCAL bit and is used to control the SCXI-1321 shunt calibration switch. CMOS/TTL output; not protected.
C6, C8	RSVD	Reserved – These pins are reserved. Do not connect any signal to these pins.
A8, C10, C16, C22, C28	No Connect	<i>Do not</i> connect any signal to these pins.
A10	EGND3	Excitation Ground 3 – This pin connects to the excitation ground 3 via a 51 k Ω resistor.
A12	EX3+	Positive Excitation Output 3 – This pin is connected to the excitation channel 3 positive output.
C12	EX3-	Negative Excitation Output 3 – This pin is connected to the excitation channel 3 negative output.
A14	CH3+	Positive Input Channel 3 – This pin is connected to the input channel 3 positive input.
C14	CH3-	Negative Input Channel 3 – This pin is connected to the input channel 3 negative input.
A16	EGND2	Excitation Ground 2 – This pin connects to the excitation ground 2 via a 51 k Ω resistor.

Pin	Signal Name	Description (continued)
A18	EX2+	Positive Excitation Output 2 – This pin is connected to the excitation channel 2 positive output.
C18	EX2-	Negative Excitation Output 2 – This pin is connected to the excitation channel 2 negative output.
A20	CH2+	Positive Input Channel 2 – This pin is connected to the input channel 2 positive input.
C20	CH2-	Negative Input Channel 2 – This pin is connected to the input channel 2 negative input.
A22	EGND1	Excitation Ground 1 – This pin connects to the excitation ground 1 via a 51 k Ω resistor.
A24	EX1+	Positive Excitation Output 1 – This pin is connected to the excitation channel 1 positive output.
C24	EX1-	Negative Excitation Output 1 – This pin is connected to the excitation channel 1 negative output.
A26	CH1+	Positive Input Channel 1 – This pin is connected to the input channel 1 positive input.
C26	CH1-	Negative Input Channel 1 – This pin is connected to the input channel 1 negative input.
A28	EGND0	Excitation Ground 0 – This pin connects to the excitation ground 0 via a 51 k Ω resistor.
A30	EX0+	Positive Excitation Output 0 – This pin is connected to the excitation channel 0 positive output.
C30	EX0-	Negative Excitation Output 0 – This pin is connected to the excitation channel 0 negative output.
A32	CH0+	Positive Input Channel 0 – This pin is connected to the input channel 0 positive input.
C32	CH0-	Negative Input Channel 0 – This pin is connected to the input channel 0 negative input.

The signals on the front connector are all analog except pins A6, C6, and C8, which are digital controls. These analog signals can be divided into three groups—the analog input channels, the excitation channels, and the temperature sensor.

Analog Input Channels

The positive input channels are located in column A. Their corresponding negative input channels are located in column C. Each input corresponds to a separate amplifier and is fully isolated from the other channels and from earth ground. The inputs are designed in a floating single-ended configuration, hence the measured signal can be referenced to a ground level with common-mode voltage up to 250 V_{rms}. For better noise immunity, connect the negative input channel to the signal reference. If the measured signals are floating, connect the negative input channel to chassis ground on the terminal block. Figure 2-4 shows how to connect a ground-referenced signal. Figure 2-5 shows how to connect a floating signal. Figures 2-6 and 2-7 show how to connect AC-coupled signals.

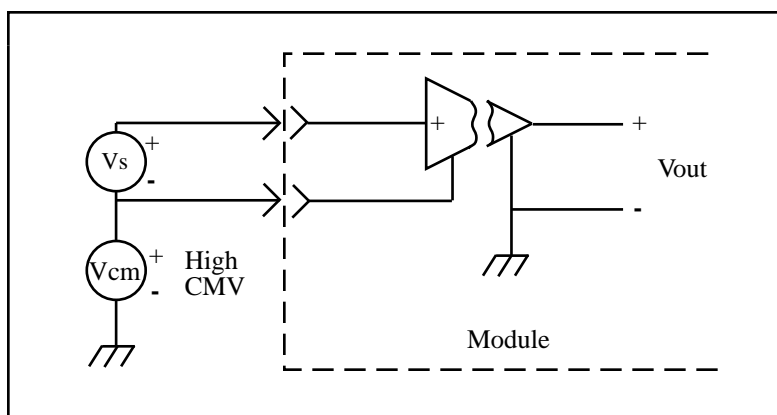


Figure 2-4. Ground-Referenced Signal Connection with High Common-Mode Voltage

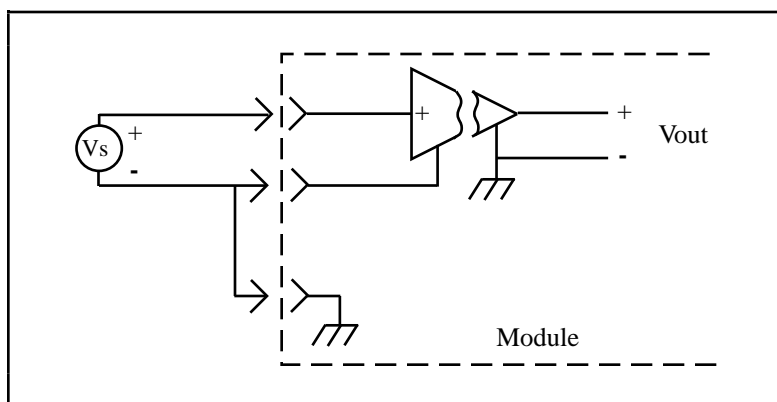


Figure 2-5. Floating Signal Connection Referenced to Chassis Ground for Better Signal-to-Noise Ratio

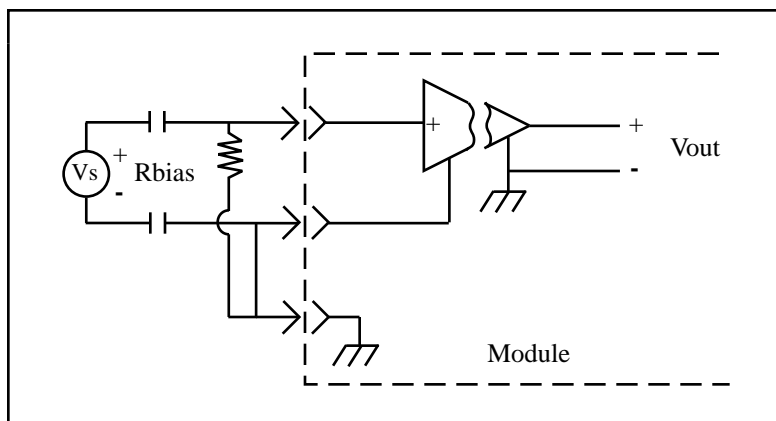


Figure 2-6. Floating AC-Coupled Signal Connection

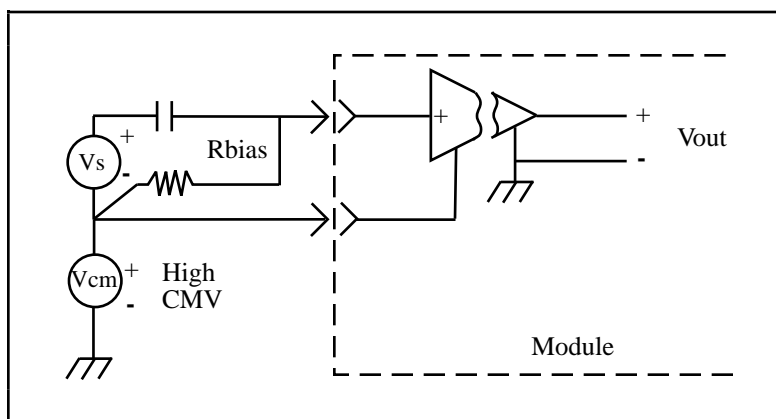


Figure 2-7. AC-Coupled Signal Connection with High Common-Mode Voltage

For AC-coupled signals, you should connect an external resistor from the positive input channel to the signal reference. This is needed to provide the DC path for the positive input bias current. Typical resistor values range from 100 kΩ to 1 MΩ. This solution, although necessary in this case, lowers the input impedance of the input channel amplifier and introduces an additional offset voltage proportional to the input bias current and to the resistor value used. The typical input bias current of the amplifier consists of ±80 pA and a negligible offset drift current. When a 100 kΩ resistor is used, this will result into ±8 μV of offset, which is insignificant in most applications. However, if larger resistors are used, significant input offset may result. To determine the maximum offset introduced by the biasing resistor, use the following equation:

$$V_{\text{offset}} = I_{\text{bias}} \times R_{\text{bias}}$$

The input signal range of an SCXI-1121 input channel is ±5 V/ G_{total} referenced to its negative input, where G_{total} is equal to the product of the first-stage and second-stage gains. In addition, the input channels are overvoltage protected to 250 Vrms with power on or off at a maximum of 4.5 mArms sink or source.

Warning: *Exceeding the input signal range and the common-mode input range results in distorted signals. Exceeding the maximum input voltage rating (250 Vrms between positive and negative terminals and between any terminal and earth ground) can damage the SCXI-1121, the SCXIbus, and the DAQ board. National Instruments is NOT liable for any damages or injuries resulting from such signal connections.*

Excitation Channels

Four fully isolated excitation channels are available. Each excitation channel corresponds to an input channel. A 250 Vrms isolation barrier exists between two corresponding channels (for example, between input channel 0 and excitation channel 0). In addition, the excitation outputs are overvoltage protected to 250 Vrms with current foldback.

Warning: *Exceeding the overvoltage protection or isolation rating on the excitation output can damage the SCXI-1121, the SCXIbus, and the DAQ board. National Instruments is NOT liable for any damages or injuries resulting from such signal connections.*

Temperature Sensor Connection

Pins C2 and C4 are dedicated for connecting the temperature sensor to the SCXI-1121. The temperature sensor is not isolated and is referenced to chassis ground. The connection is overvoltage-protected to ± 25 VDC with power on and ± 15 VDC with power off.

Warning: *Exceeding the overvoltage protection on the temperature connections can damage the SCXI-1121, the SCXIbus, and the DAQ board. National Instruments is NOT liable for any damages resulting from such signal connections.*

Connector-and-Shell Assembly

Two types of signal connectors are available to connect the transducers to the SCXI-1121 inputs. The first, the SCXI-1330 32-pin DIN C female connector-and-shell assembly, is available in a kit listed in the *Optional Equipment* section in Chapter 1, *Introduction*. The connector has eyelet ends for easy hook-and-solder wire connection. With this kit, you can build your own signal cable to connect to the SCXI-1121 inputs. After you have built the cable, the shell covers and protects the connector. Perform the following steps to assemble and mount the connector-and-shell assembly to your SCXI module:

1. Refer to Figure 2-8, *Assembling and Mounting the SCXI-1330 Connector-and-Shell Assembly*, and the diagram included with your SCXI-1330 kit to build the connector-and-shell assembly.
2. Turn off the computer that contains your DAQ board or disconnect the board from your SCXI chassis.
3. Turn off your SCXI chassis.
4. Slide the selected module out of the SCXI chassis.
5. Remove the module cover.

6. Place one jack screw on the SCXI-1121 as indicated in Figure 2-8.
7. While holding the jack screw in place, insert the lock washer and then the nut. Notice that you might need long-nose pliers to insert the washer and nut.
8. Tighten the nut by holding it firmly and rotating the jack screw.
9. Repeat steps 6 through 8 for the second jack screw.
10. Replace the module cover and tighten the grounding screw.
11. Slide the module back in place.
12. Connect the SCXI-1330 to your module connector and secure it by tightening both mounting screws.

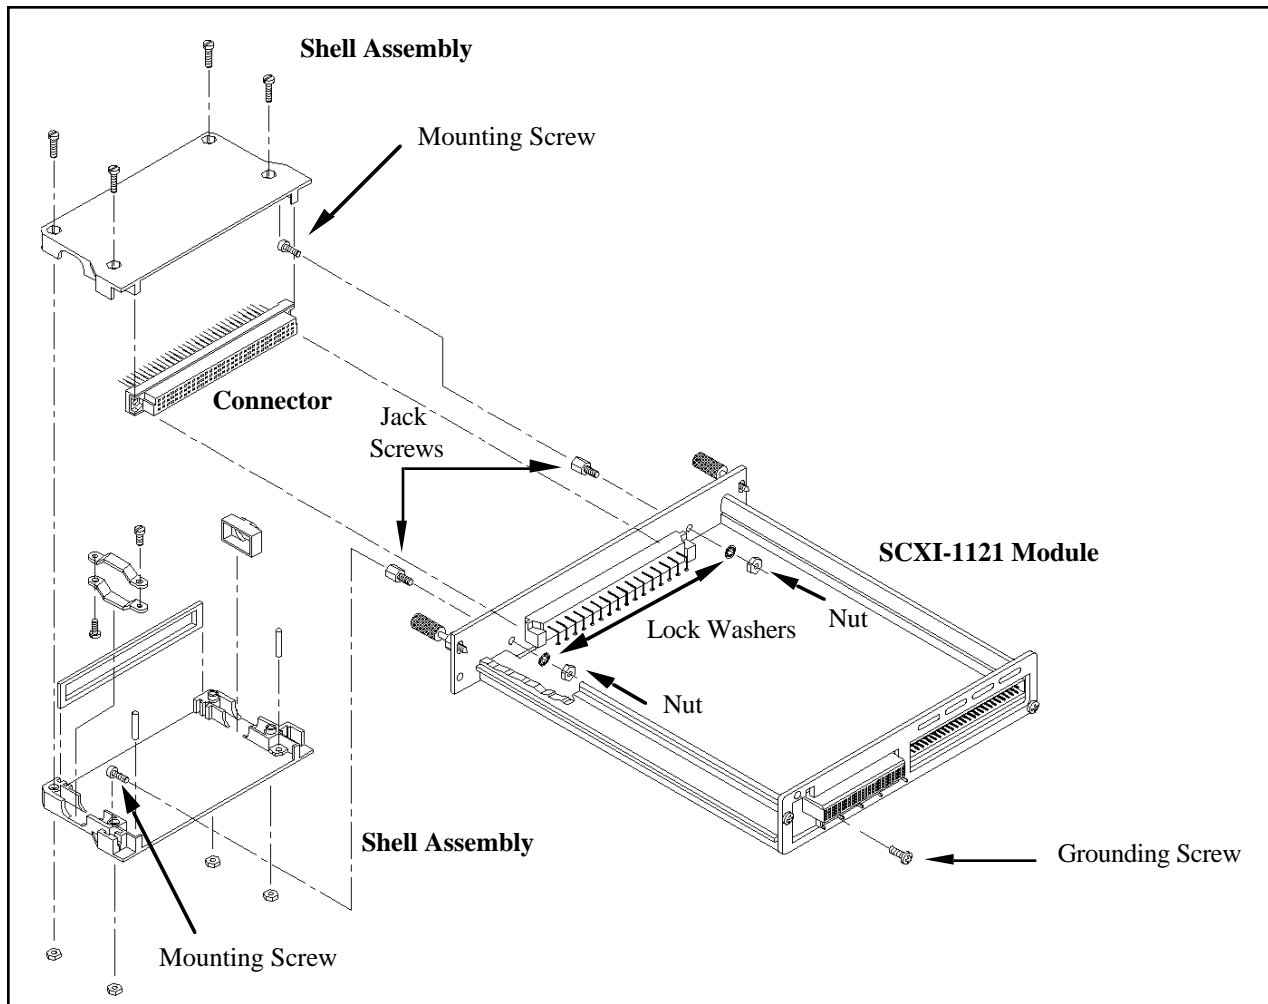


Figure 2-8. Assembling and Mounting the SCXI-1330 Connector-and-Shell Assembly

SCXI-1320, SCXI-1328, and SCXI-1321 Terminal Blocks

The second type of connector available to connect the transducers to the SCXI-1121 inputs is a terminal block with an onboard temperature sensor and screw terminals for easy connection. One terminal block, the SCXI-1328 isothermal terminal block, has a high-accuracy onboard temperature sensor. The terminal block kits are listed in the *Optional Equipment* section in Chapter 1, *Introduction*.

The terminal blocks consist of a shielded board with supports for connection to the SCXI-1121 input connector. The terminal blocks have 18 screw terminals for easy connection. Four pairs of screw terminals are for signal connection to the four inputs of the SCXI-1121, four pairs are for the excitation channels, and one pair of screw terminals connects to the chassis ground.

The following warnings contain important safety information concerning hazardous voltages and terminal blocks.

Warnings: *When using the terminal block with high common-mode voltages, you must insulate your signal wires appropriately. National Instruments is NOT liable for any damages or injuries resulting from inadequate signal wire insulation.*

If high voltages (≥ 42 Vrms) are present, you must connect the safety earth ground to the strain-relief tab. This complies with UL 1244 and protects against electric shock when the terminal block is not connected to the chassis. To connect the safety earth ground to the strain-relief tab, run an earth ground wire in the cable from the signal source to the terminal block. National Instruments is NOT liable for any damages or injuries resulting from inadequate safety earth ground connections.

SCXI-1320 and SCXI-1328 Terminal Blocks

When connecting your signals to the SCXI-1320 terminal block for use with the SCXI-1121, follow the labeling on the SCXI-1320 indicated under the module type column for the SCXI-1121 as indicated in Figure 2-11.

When connecting your signals to the SCXI-1328 high-accuracy isothermal terminal block for use with the SCXI-1121, follow the labeling on the SCXI-1328 indicated along the module type row for the SCXI-1121 as indicated in Figure 2-12.

SCXI-1321 Offset-Null and Shunt-Calibration Terminal Block

The SCXI-1321 terminal block operates only with Revision C and later SCXI-1121 modules.

In addition to the 18 screw terminals, the SCXI-1321 has circuitry for offset-null adjust of Wheatstone bridges as well as a shunt resistor for strain-gauge shunt calibration. This terminal block works especially well with bridge-type transducers such as strain gauges. The SCXI-1321 can also easily accommodate thermocouples, RTDs, thermistors, millivolt sources, volt sources, and current-loop receivers.

SCXI-1321 Nulling Circuitry. The nulling circuitry operates with full-bridge, half-bridge, quarter-bridge, and strain-gauge configurations. Each channel has its own nulling circuitry and its own trimming potentiometer as listed in Table 2-10.

Table 2-10. Trimmer Potentiometer and Corresponding Channel

Channel Number	Trimmer Potentiometer
0	R1
1	R2
2	R14
3	R15

To null the static offset voltage of the bridge, use the following procedure:

1. Configure your bridge to the selected channel.
2. Select and read the channel output.
3. While monitoring the output, rotate the trimmer wiper with a flathead screwdriver until you reach 0 V.

You have nulled your bridge and are ready for a measurement.

The nulling range for your terminal block is ± 2.5 mV, assuming that you have a 120Ω strain gauge and 3.333 V excitation voltage. You can change this range by replacing the nulling resistor with a resistor of another value. Each channel has an independent nulling resistor. You can therefore mix your ranges to accommodate each channel requirement. Table 2-11 lists the nulling resistors and their corresponding channels.

Table 2-11. Nulling Resistors and Corresponding Channel

Channel Number	Nulling Resistor
0	R3
1	R5
2	R7
3	R9

The value of all the nulling resistors on your terminal block is 39 k Ω . Notice that these resistors are socketed for easy replacement. These sockets best fit a 1/4 W resistor lead size.

To determine your nulling range, use the following formula (refer to Figure 2-9 for visual help):

$$V_{\text{nulling range}} = \pm \left| \frac{V_{\text{exc}}}{2} - \frac{V_{\text{exc}} R_d (R_{\text{null}} + R_g)}{R_{\text{null}} R_g + R_d (R_{\text{null}} + R_g)} \right|$$

where

R_g is the nominal strain-gauge resistance value.

R_d is either a completion resistor or a second strain-gauge nominal resistance.

R_{null} is the nulling resistor value.

V_{exc} is the excitation voltage (3.333 or 10 V).

For example, assuming:

$$V_{\text{exc}} = 3.333 \text{ V}$$

$$R_g = 120 \ \Omega$$

$$R_d = 120 \ \Omega$$

$$R_{\text{null}} = 39 \text{ k}\Omega$$

$$V_{\text{nulling}} = \pm 2.56 \text{ mV}$$

Assuming a strain-gauge range with a gauge factor of $GF = 2$ and a quarter-bridge configuration, this range corresponds to $\pm 1,498 \ \mu\epsilon$ as given by the strain formula for a quarter-bridge strain-gauge configuration:

$$\epsilon = \frac{-4V_r}{GF(1 + 2V_r)}$$

where

$$V_r = \frac{\text{strained voltage} - \text{static unstrained voltage}}{V_{\text{exc}}}$$

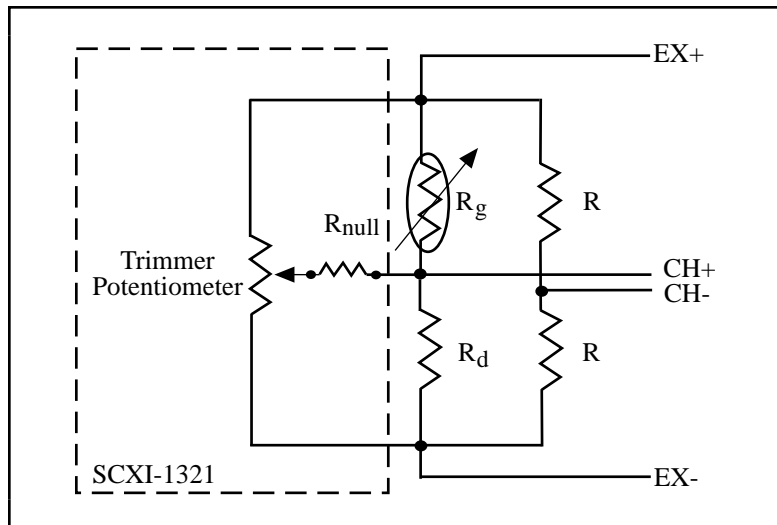










Figure 2-9. Nulling Circuit

Using the SCXI-1321 with RTDs and Thermistors. When using this terminal block with RTDs or thermistor-type transducers and with the SCXI-1121 excitation set in the Current mode, you must disable the nulling circuit of the channel of interest. You can do this in two steps:

1. Place the enable/disable jumper in position D (disable) as shown in Table 2-12.
2. Remove the nulling resistor from its sockets.

Table 2-12. Jumper Settings of the Nulling Circuits

Jumper	Position	Description
W1		Nulling circuit of Channel 0 is enabled; factory setting
		Nulling circuit of Channel 0 is disabled
W2		Nulling circuit of Channel 1 is enabled; factory setting
		Nulling circuit of Channel 1 is disabled
W3		Nulling circuit of Channel 2 is enabled; factory setting
		Nulling circuit of Channel 2 is disabled
W4		Nulling circuit of Channel 3 is enabled; factory setting
		Nulling circuit of Channel 3 is disabled

SCXI-1121 Shunt Calibration. Shunt calibration circuits are independent from each other but are controlled together. In other words, when SCAL is set to 1 on the SCXI-1121, all the shunt switches close; when SCAL is cleared to 0, all the switches open. At startup or reset, all switches are open. This shunt calibration circuitry configuration places a shunting resistor in parallel with the strain gauge as shown in Figure 2-10.

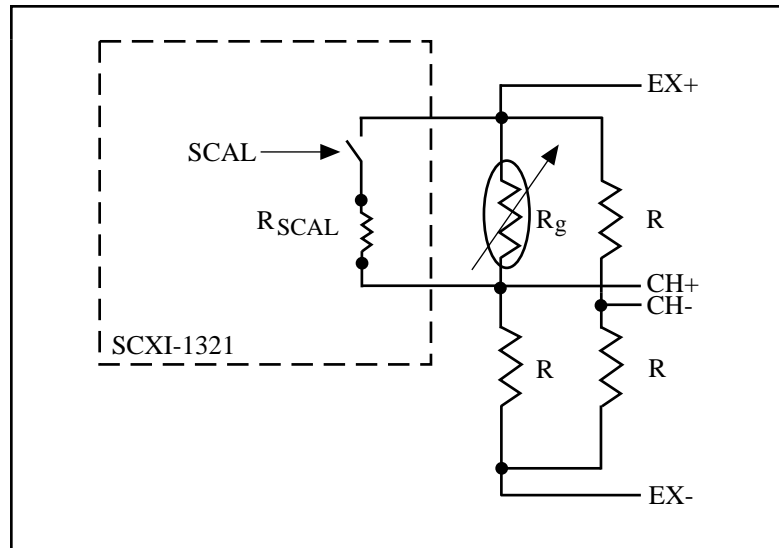


Figure 2-10. Shunt Circuit

The shunting resistors R_{SCAL} are socketed so that you can replace them with a resistor of another value to achieve the required changes. The R_{SCAL} resistors on your terminal block have a $301\text{ k}\Omega \pm 1\%$ value.

Assuming a quarter-bridge strain-gauge configuration with a gauge factor of $GF = 2$, the equivalent strain change introduced by the R_{SCAL} shunting resistor is $-199\text{ }\mu\epsilon$. Determine the change as follows:

1. Determine the change caused by the shunting resistor using the following formula:

$$V_{\text{change}} = \frac{V_{\text{exc}} R_d (R_{SCAL} + R_g)}{R_{SCAL} + R_d (R_{SCAL} + R_g)} - \frac{V_{\text{exc}}}{2}$$

2. Using the appropriate strain-gauge strain formula, and assuming that you have no static voltage, determine the equivalent strain that the R_{SCAL} should produce. For example, $R_{SCAL} = 301\text{ k}\Omega$ and a quarter-bridge $120\text{ }\Omega$ strain gauge with a gauge factor of $GF = 2$ and $V_{\text{exc}} = 3.333\text{ V}$ and $R = 120\text{ }\Omega$ produces the following result:

$$V_{\text{change}} = 0.3321\text{ mV}$$

Replacing the strained voltage with V_{change} in the quarter-bridge strain equation produces an equivalent $-199\text{ }\mu\epsilon$ of change.

Terminal Block Temperature Sensor

To accommodate thermocouples with the SCXI-1121, the terminal block has an onboard temperature sensor for cold-junction compensation. You can connect this temperature sensor in two ways:

- You can connect the temperature sensor to the MTEMP pin (C4) on the module front connector and multiplex the sensor at the output multiplexer along with the amplifier outputs. This is the Multiplexed Temperature Sensor (MTS) mode. Refer to the *Configuration Register* section in Chapter 4, *Register Descriptions*, for further details.
- You can connect the temperature sensor to a separate data acquisition channel via MCH4± (pins 11 and 12 on the module rear signal connector). This is the Direct Temperature Sensor (DTS) mode.

Note: *Use an average of a large number of samples to obtain the most accurate reading. Noisy environments require more samples for greater accuracy.*

The SCXI-1320 and SCXI-1321 temperature sensors output 10 mV/°C and have an accuracy of ±1° C over the 0° to 55° C temperature range. To determine the temperature, use the following formulas:

$$T (^{\circ}\text{C}) = 100(V_{\text{TEMPOUT}})$$

$$T (^{\circ}\text{F}) = \frac{[T (^{\circ}\text{C})] 9}{5} + 32$$

where V_{TEMPOUT} is the temperature sensor output and $T (^{\circ}\text{F})$ and $T (^{\circ}\text{C})$ are the temperature readings in degrees Fahrenheit and degrees Celsius, respectively.

The SCXI-1328 temperature sensor outputs 0.62 to 0.07 V from 0° to 55° C and has an accuracy of ±0.35° C over the 15° to 35° C range and ±0.65° C over the 0° to 15° and 35° to 55° C ranges. To determine the temperature, use the following formulas:

$$T (^{\circ}\text{C}) = T_{\text{K}} - 273.15$$

where T_{K} is the temperature in kelvin

$$T_{\text{K}} = \frac{1}{\left[a + b(\ln R_{\text{T}}) + c(\ln R_{\text{T}})^3 \right]}$$

$$a = 1.288 \times 10^{-3}$$

$$b = 2.356 \times 10^{-4}$$

$$c = 9.556 \times 10^{-8}$$

R_{T} = resistance of the thermistor in Ω

$$R_{\text{T}} = 50,000 \left(\frac{V_{\text{TEMPOUT}}}{2.5 - V_{\text{TEMPOUT}}} \right)$$

V_{TEMPOUT} = output voltage of the temperature sensor

$$T (^{\circ}\text{F}) = \frac{[T (^{\circ}\text{C})] 9}{5} + 32$$

where $T (^{\circ}\text{F})$ and $T (^{\circ}\text{C})$ are the temperature readings in degrees Fahrenheit and degrees Celsius, respectively.

Terminal Block Jumper Configuration

In addition to the screw terminals, the terminal block has one jumper for configuring the onboard temperature sensor. When you set jumper W1 on the SCXI-1320 or SCXI-1328 (jumper W5 on the SCXI-1321) to the MTEMP position, the jumper connects the temperature sensor output to the SCXI-1121 output multiplexer. This is the factory setting. The DTEMP position of jumper W1 (jumper W5 on the SCXI-1321) connects the temperature sensor to the SCXI-1121 MCH4+ signal on the rear signal connector.

In both MTS and DTS modes, the reference to the temperature sensor signal is the SCXI-1121 analog ground that is connected to MCH0- in the MTS mode and to MCH4- in the DTS mode. Notice that MCH4- is continuously connected to the SCXI-1121 ground, whereas MCH0- is switched through the output multiplexer.

One jumper block comprises both positions; thus, you can use only one type of configuration at a time. The parking position for the jumper block is in the MTEMP position (the temperature sensor is disabled until the RTEMP bit in the Configuration Register selects the sensor).

Tables 2-13, 2-14, and 2-15 show the jumper settings on the SCXI-1320, SCXI-1328, and SCXI-1321 terminal blocks.

Table 2-13. Jumper Settings on the SCXI-1320 Terminal Block





Jumper	Position	Description
W1	 MTEMP  DTEMP	MTS mode selected; factory setting; parking position
W1	 MTEMP  DTEMP	DTS mode selected

Table 2-14. Jumper Settings on the SCXI-1328 Terminal Block





Jumper	Position	Description
W1	 MTEMP DTEMP	MTS mode selected; factory setting; parking position
W1	 DTEMP MTEMP	DTS mode selected

Table 2-15. Jumper Settings on the SCXI-1321 Terminal Block

Jumper	Position	Description
W5		MTS mode selected; factory setting; parking position
W5		DTS mode selected

Terminal Block Signal Connection

Warnings: *The chassis GND terminals on your terminal block are for grounding high impedance sources such as a floating source (1 mA maximum). Do NOT use these terminals as safety earth grounds.*

If high voltages (≥ 42 Vrms) are present, you must connect the safety earth ground to the strain-relief tab. This complies with UL 1244 and fully protects against electric shock when the terminal block is not connected to the chassis. To connect the safety earth ground to the strain-relief tab, run an earth ground wire in the cable from the signal source to the terminal block. National Instruments is NOT liable for any damages or injuries resulting from inadequate safety earth ground connections.



Shock Hazard: *This unit should only be opened by qualified personnel aware of the dangers involved. Disconnect all power before removing cover. Always install grounding screw.*

To connect the signal to the terminal block, use the following procedure:

1. Remove the grounding screw of the top cover.
2. Snap out the top cover of the shield by placing a screwdriver in the groove at the bottom of the terminal block.
3. Slide the signal wires, one at a time, through the front panel strain-relief opening. You can add padding or insulation if necessary.
4. Connect the wires to the screw terminals. For thermistor and RTD connection, follow the procedure stated in the *Using the SCXI-1321 with RTDs and Thermistors* section earlier in this chapter.
5. Tighten the larger strain-relief screws.
6. Snap the top cover back in place.
7. Reinsert the grounding screw to ensure proper shielding.
8. Connect the terminal block to the SCXI-1121 front connector as explained in the *Terminal Block Installation* section later in this chapter.

Figure 2-11 shows a parts locator diagram for the SCXI-1320 terminal block. Figure 2-12 shows a parts locator diagram for the SCXI-1328 terminal block. Figure 2-13 shows a parts locator diagram for the SCXI-1321 terminal block.




Figure 2-11. SCXI-1320 Parts Locator Diagram



Figure 2-12. SCXI-1328 Parts Locator Diagram



Figure 2-13. SCXI-1321 Parts Locator Diagram

Terminal Block Installation

To connect the terminal block to the SCXI-1121 front connector, perform the following steps:

1. Connect the SCXI-1121 front connector to its mating connector on the terminal block.
2. Make sure that the SCXI-1121 top and bottom thumbscrews do not obstruct the rear panel of the terminal block.
3. Tighten the top and bottom screws on the back of the terminal block to hold it securely in place.

Rear Signal Connector

Note: *If you are using the SCXI-1121 with a National Instruments data acquisition board and cable assembly, you do not need to read the remainder of this chapter. If you are using the SCXI-1180 feedthrough panel, the SCXI-1343 rear screw terminal adapter, or the SCXI-1351 one-slot cable extender with the SCXI-1121, you should read this section.*

Figure 2-14 shows the pin assignments for the SCXI-1121 rear signal connector.

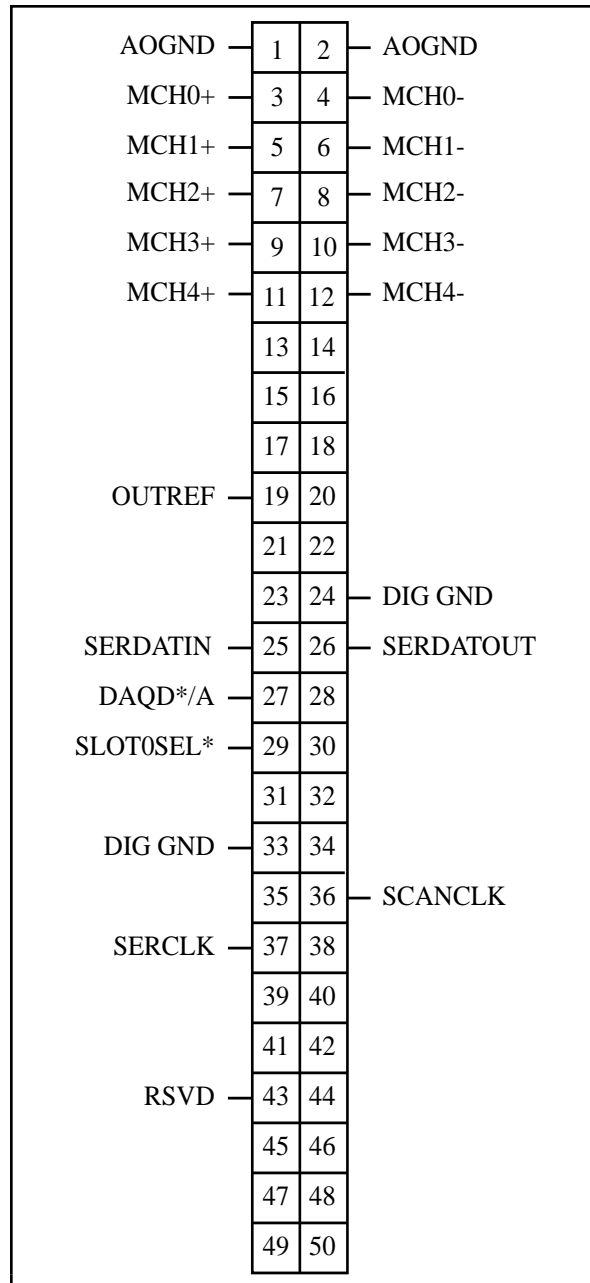


Figure 2-14. SCXI-1121 Rear Signal Connector Pin Assignment

Rear Signal Connector Signal Descriptions

Pin	Signal Name	Description
1-2	AOGND	Analog Output Ground – These pins are connected to the analog reference when jumper W33 is in position AB-R0.
3-12	MCH0± through MCH4±	Analog Output Channels 0 through 4 – Connects to the data acquisition board differential analog input channels.
19	OUTREF	Output Reference – This pin serves as the reference node for the analog channels output in the Pseudodifferential Reference mode. It should be connected to the analog input sense of the NRSE data acquisition board.
24, 33	DIG GND	Digital Ground – These pins supply the reference for data acquisition board digital signals and are tied to the module digital ground.
25	SERDATIN	Serial Data In – This signal taps into the SCXIBus MOSI line to provide serial input data to a module or Slot 0.
26	SERDATOUT	Serial Data Out – This signal taps into the SCXIBus MISO line to accept serial output data from a module.
27	DAQD*/A	Data Acquisition Board Data/Address Line – This signal taps into the SCXIBus D*/A line to indicate to the module whether the incoming serial stream is data or address information.
29	SLOT0SEL*	Slot 0 Select – This signal taps into the SCXIBus INTR* line to indicate whether the information on MOSI is being sent to a module or Slot 0.
36	SCANCLK	Scan Clock – This indicates to the SCXI-1121 that a sample has been taken by the data acquisition board and causes the SCXI-1121 to change channels. See the <i>Timing Requirements and Communication Protocol</i> section later in this chapter for more detailed information on timing.
37	SERCLK	Serial Clock – This signal taps into the SCXIBus SPICLK line to clock the data on the MOSI and MISO lines. See the <i>Timing Requirements and Communication Protocol</i> section later in this chapter for more detailed information on timing.
43	RSVD	Reserved.

All other pins are not connected.

The signals on the rear signal connector can be classified as analog output signals, digital I/O signals, or timing I/O signals. Signal connection guidelines for each of these groups are given in the following section.

Analog Output Signal Connections

Pins 1 through 12 and pin 19 of the rear signal connector are analog output signal pins. Pins 1 and 2 are AOGND signal pins. AOGND is an analog output common signal that is routed through jumper W33 to the analog reference on the SCXI-1121. You can use these pins for a general analog power ground tie point to the SCXI-1121 if necessary. In particular, when using differential input data acquisition boards such as the MIO-16 series, it is preferable to leave jumper W33 in its factory setting or in position AB-R1 to avoid ground loops. With data acquisition boards that are configured for referenced single-ended (RSE) measurements, W33 should be in position AB-R0 to connect the SCXI-1121 ground to the data acquisition analog ground. Pin 19 is the OUTREF pin; this pin is connected internally to the analog reference when jumper W33 is in position AB-R2. Pins 3 through 12 are the analog output channels of the SCXI-1121. Pins 3 and 4 or MCH0± are a multiplexed output of all four input channels and the temperature sensor output. Pins 5 through 10 or MCH1± through MCH3± are a parallel connection of input channels 1 through 3 to the rear signal connector. Pins 11 and 12 or MCH4± are a direct connection of the temperature sensor. Notice that the temperature sensor is located on the terminal block. For further details on configuring the temperature sensor output, refer to the *SCXI-1320, SCXI-1328, and SCXI-1321 Terminal Blocks* section earlier in this chapter.

Warning: *The SCXI-1121 analog outputs are not overvoltage-protected. Applying external voltages to these outputs can damage the SCXI-1121. National Instruments is NOT liable for any damages resulting from such signal connections.*

Note: *The SCXI-1121 analog outputs are short-circuit protected.*

Digital I/O Signal Connections

Pins 24 through 27, 29, 33, 36, 37, and 43 constitute the digital I/O lines of the rear signal connector. They are divided into three categories—the digital input signals, the digital output signals, and the digital timing signals.

The digital input signals are pins 24, 25, 27, 29, 33, and 37. The data acquisition board uses these pins to configure an SCXI module that is under data acquisition board control. Each digital line emulates the SCXibus communication signals as follows.

- Pin 25 is SERDATIN and is equivalent to the SCXibus MOSI serial data input line.
- Pin 27 is DAQD*/A and is equivalent to the SCXibus D*/A line. It indicates to the module whether the incoming serial stream on SERDATIN is data (DAQD*/A = 0), or address (DAQD*/A = 1) information.
- Pin 29 is SLOT0SEL* and is equivalent to the SCXibus INTR* line. It indicates whether the data on the SERDATIN line is being sent to Slot 0 (SLOT0SEL* = 0) or to a module (SLOT0SEL* = 1).

Digital output specifications (referenced to DIG GND):

V_{OH} output logic high voltage	3.7 V minimum at 4 mA maximum
V_{OL} output logic low voltage	0.4 V maximum at 4 mA maximum

Timing Requirements and Communication Protocol

Timing Signal

The data acquisition timing signal is SCANCLK.

SCANCLK is used to increment MUXCOUNTER on its rising edge. Figure 2-15 shows the timing requirements of the SCANCLK signal. These requirements will ensure that SCANCLK is properly transmitted over TRIG0.

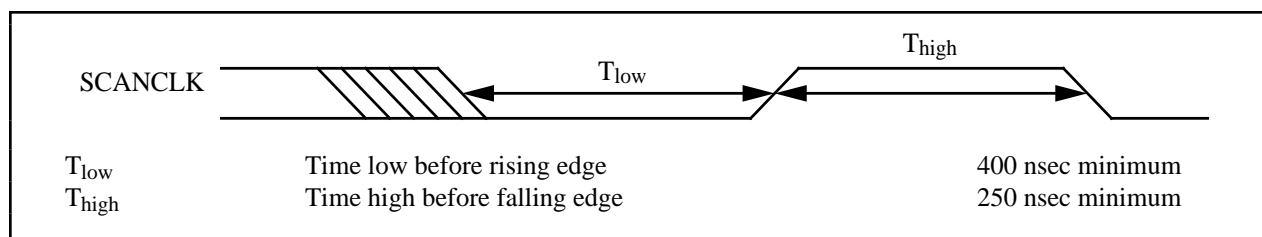


Figure 2-15. SCANCLK Timing Requirements

For output selection time specifications, refer to Appendix A, *Specifications*.

Communication Signals

This section describes the methods for communicating on the Serial Peripheral Interface (SPI) bus and their timing requirements. The communication signals are SERDATIN, DAQD*/A, SLOT0SEL*, SERDATOUT, and SERCLK. Furthermore, SS* is produced by Slot 0 according to data acquisition board programming, and SS* timing relationships will also be discussed. For information on the Slot 0 Slot-Select Register, consult Chapter 4, *Register Descriptions*.

The data acquisition board determines to which slot it will talk by writing a slot-select number to Slot 0. In the case of an SCXI-1001 chassis, this write also determines to which chassis the data acquisition board will talk. Writing a slot-select number is also used in programming the Slot 0 hardscan circuitry. See Chapter 5, *Programming*, for information on programming the Slot 0 hardscan circuitry.

The following sections detail the procedure for selecting a slot in a particular chassis. Figure 2-16 illustrates the timing of this procedure with the example case of selecting Slot 11 in Chassis 9. Notice that the factory-default chassis address for the SCXI-1000 is address 0. For information on changing the address of your chassis, consult the *SCXI-1000/1001 User Manual*. An SCXI-1000 chassis will respond to any chassis number.

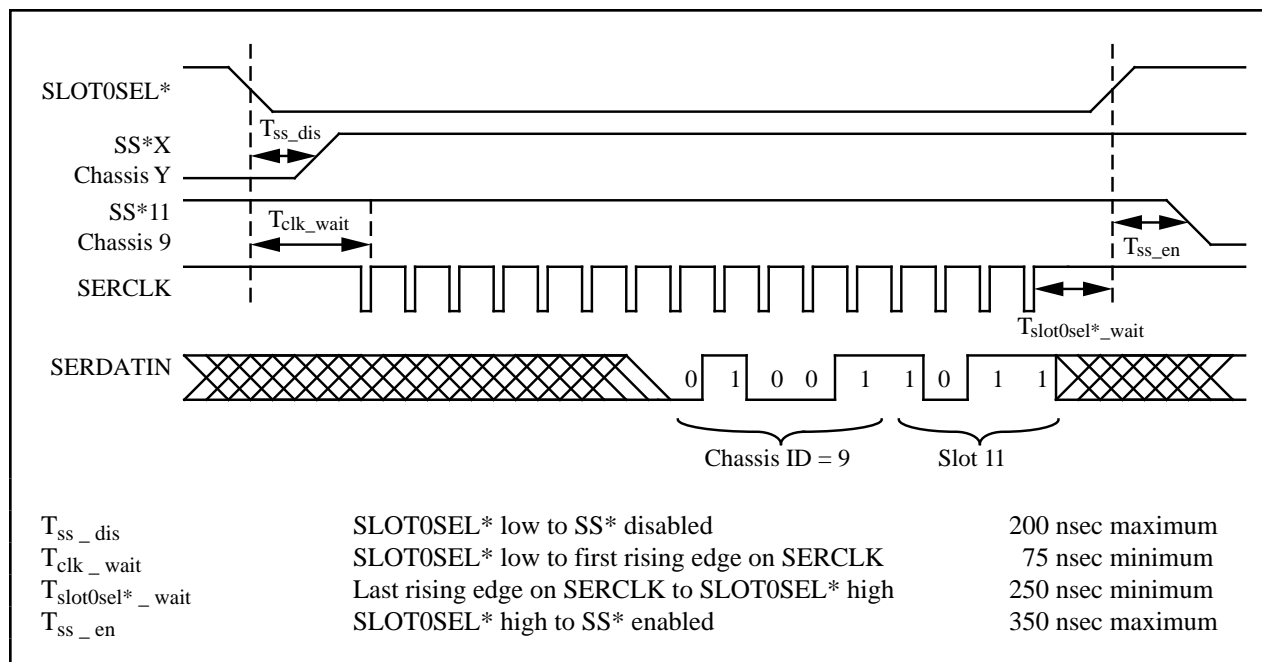


Figure 2-16. Slot-Select Timing Diagram

To write the 16-bit slot-select number to Slot 0, follow these steps:

1. Initial conditions:

SERDATIN = don't care
 DAQD*/A = don't care
 SLOTOSEL* = 1
 SERCLK = 1

2. Clear SLOTOSEL* to 0. This will deassert all SS* lines to all modules in all chassis.

3. For each bit, starting with the most significant bit, perform the following action:

- a. SERDATIN = bit to be sent. These bits are the data that is being written to the Slot-Select Register.
- b. SERCLK = 0
- c. SERCLK = 1. This rising edge clocks the data.

4. Set SLOTOSEL* to 1. This will assert the SS* line of the module whose slot number was written to Slot 0. If multiple chassis are being used, only the appropriate slot in the chassis whose address corresponds to the written chassis number will be selected. When no communication is taking place between the data acquisition board and any modules, it is recommended that 0 be written to the Slot-Select Register to ensure that no accidental writes occur.

Figure 2-17 shows the timing requirements on the SERCLK and SERDATIN signals. You must observe these timing requirements for all communications. T_{delay} is a specification of the SCXI-1121.

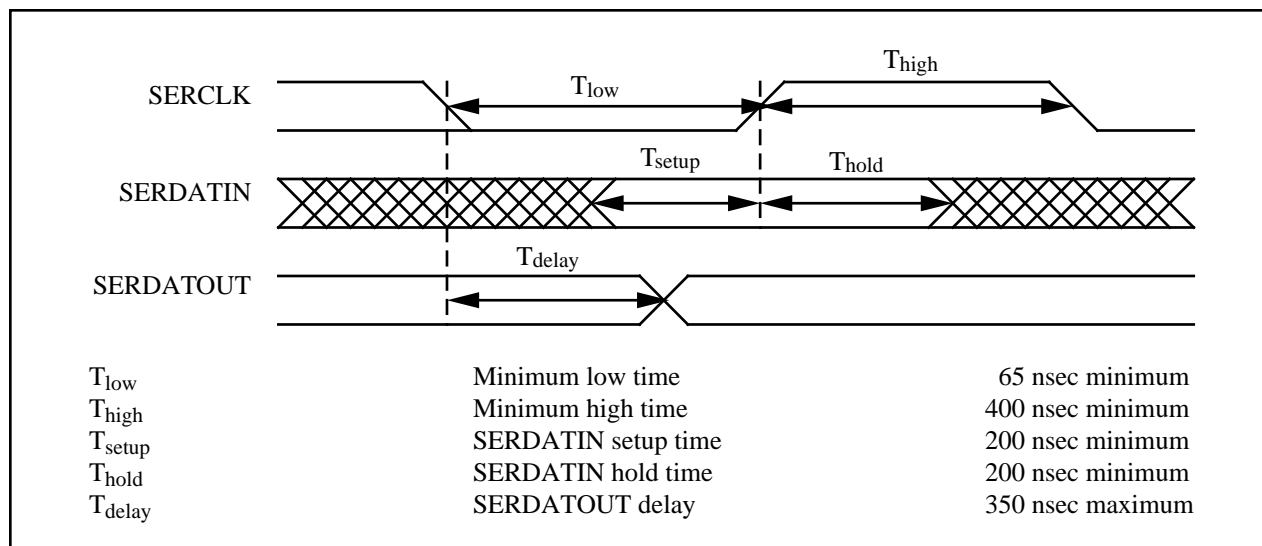


Figure 2-17. Serial Data Timing Diagram

After the Slot-Select line to an SCXI-1121 has been asserted, you can write to its Configuration Register and read from its Module ID Register by following the protocols given below. The contents of the Module ID Register are reinitialized by deasserting Slot-Select. After the 32 bits of data are read from the Module ID Register, further data will be zeros until reinitialization occurs.

To write to the Configuration Register, follow these steps:

1. Initial conditions:

SS* asserted low
 SERDATIN = don't care
 DAQD*/A = 0 (indicates data will be written to Configuration Register)
 SLOT0SEL* = 1
 SERCLK = 1 (and has not transitioned since SS* went low)

2. For each bit to be written:

Establish the desired SERDATIN level corresponding to this bit.
 SERCLK = 0
 SERCLK = 1. Clock the data.

3. Pull SLOT0SEL* low to deassert the SS* line and establish conditions for writing a new slot-select number to the Slot 0 Slot-Select Register.

4. If you are not selecting another slot, you should write zero to the Slot 0 Slot-Select Register.

Figure 2-18 illustrates a write to the SCXI-1121 Configuration Register of the binary pattern:

10000011 00001111

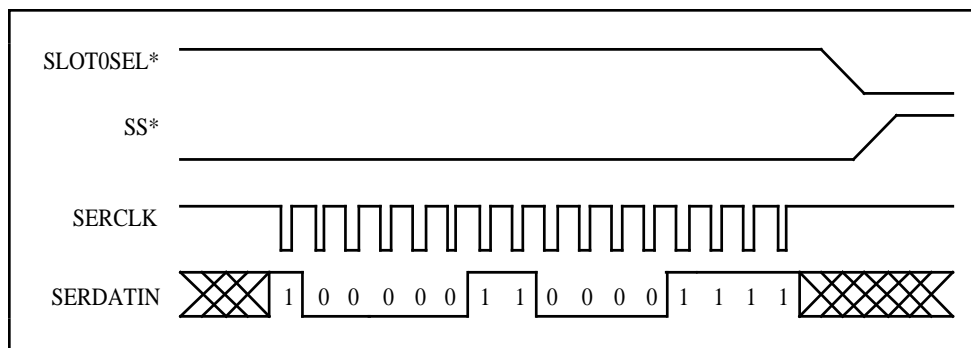


Figure 2-18. Configuration Register Write Timing Diagram

To read from the Module ID Register, follow these steps:

1. Initial conditions:

- SS* asserted low
- SERDATIN = don't care
- DAQD*/A = 1. Make sure DAQD*/A does not go low or erroneous data will be written to the Configuration Register.
- SLOTOSEL* = 1
- SERCLK = 1 (and has not changed since SS* went low)

2. For each bit to be read:

- SERCLK = 0
- SERCLK = 1. Clock the data.
- Read the level of the SERDATOUT line.

3. Pull SLOTOSEL* low to deassert the SS* line and establish conditions for writing a new slot-select number to the Slot 0 Slot-Select Register.

4. If you are not selecting another slot, you should write zero to the Slot 0 Slot-Select Register.

Figure 2-19 illustrates a read of the SCXI-1121 Module ID Register.

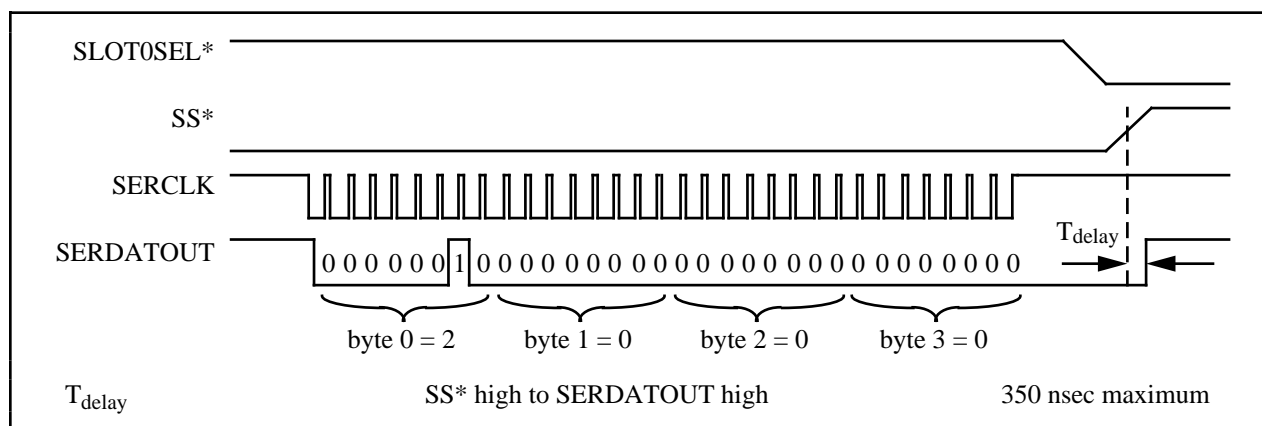


Figure 2-19. SCXI-1121 Module ID Register Timing Diagram

For further details on programming these signals, refer to Chapter 5, *Programming*.

Chapter 3

Theory of Operation

This chapter contains a functional overview of the SCXI-1121 module and explains the operation of each functional unit making up the SCXI-1121.

Functional Overview

The block diagram in Figure 3-1 illustrates the key functional components of the SCXI-1121.

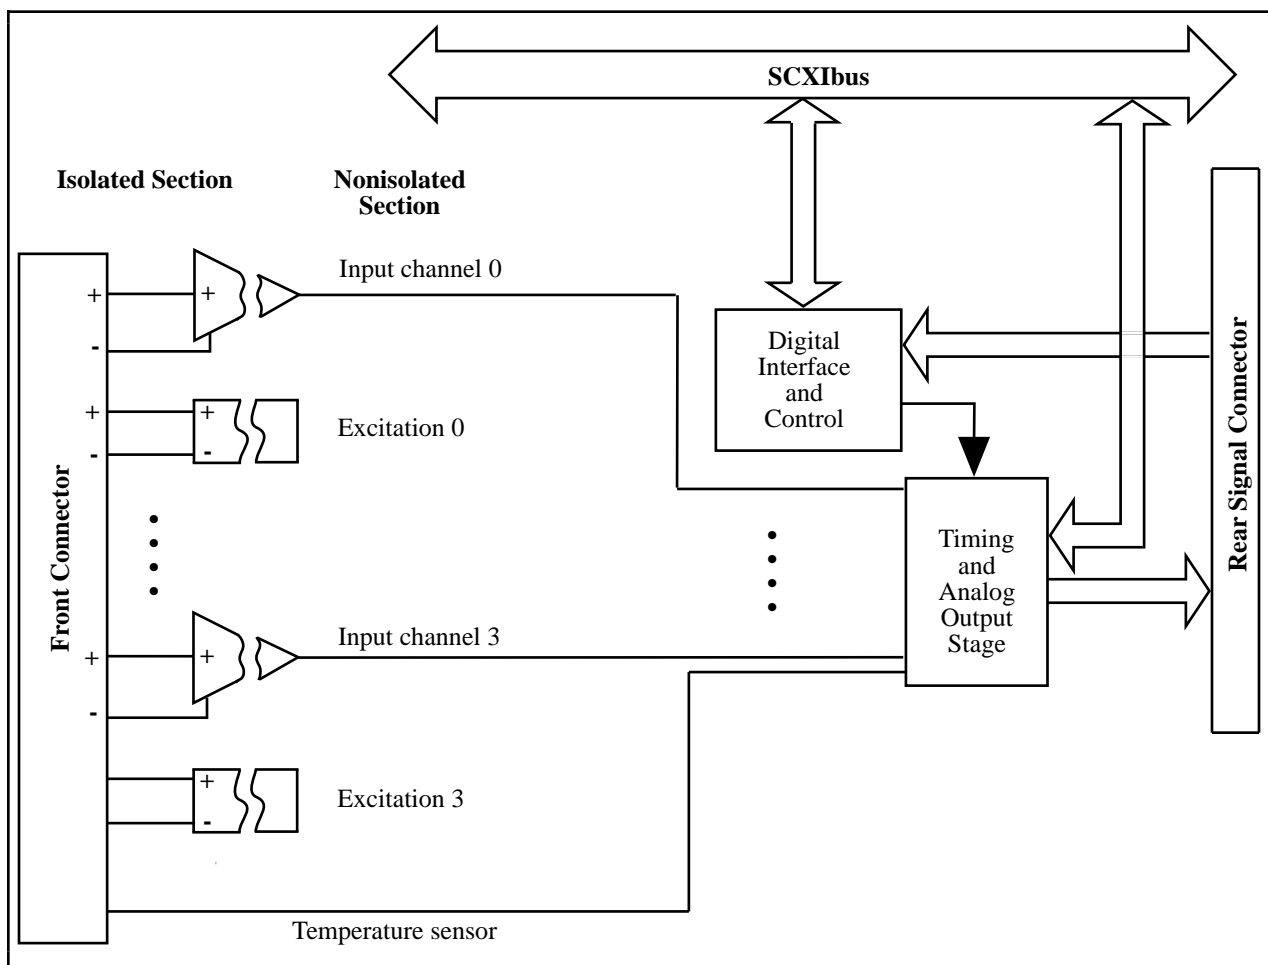


Figure 3-1. SCXI-1121 Block Diagram

The major components of the SCXI-1121 are as follows:

- SCXIbus connector
- Digital interface
- Digital control circuitry
- Timing and analog circuitry

The SCXI-1121 consists of four isolated amplifier channels with gains of 1, 2, 5, 10, 20, 50, 100, 200, 500, 1,000, and 2,000, and four isolated excitation channels with voltage or current excitation. The SCXI-1121 also has a digital section for automatic control of channel scanning, for temperature selection, and for MUXCOUNTER clock selection.

The theory of operation for each of these components is explained in the rest of this chapter.

SCXIbus Connector

Figure 3-2 shows the pin assignments for the SCXIbus connector.

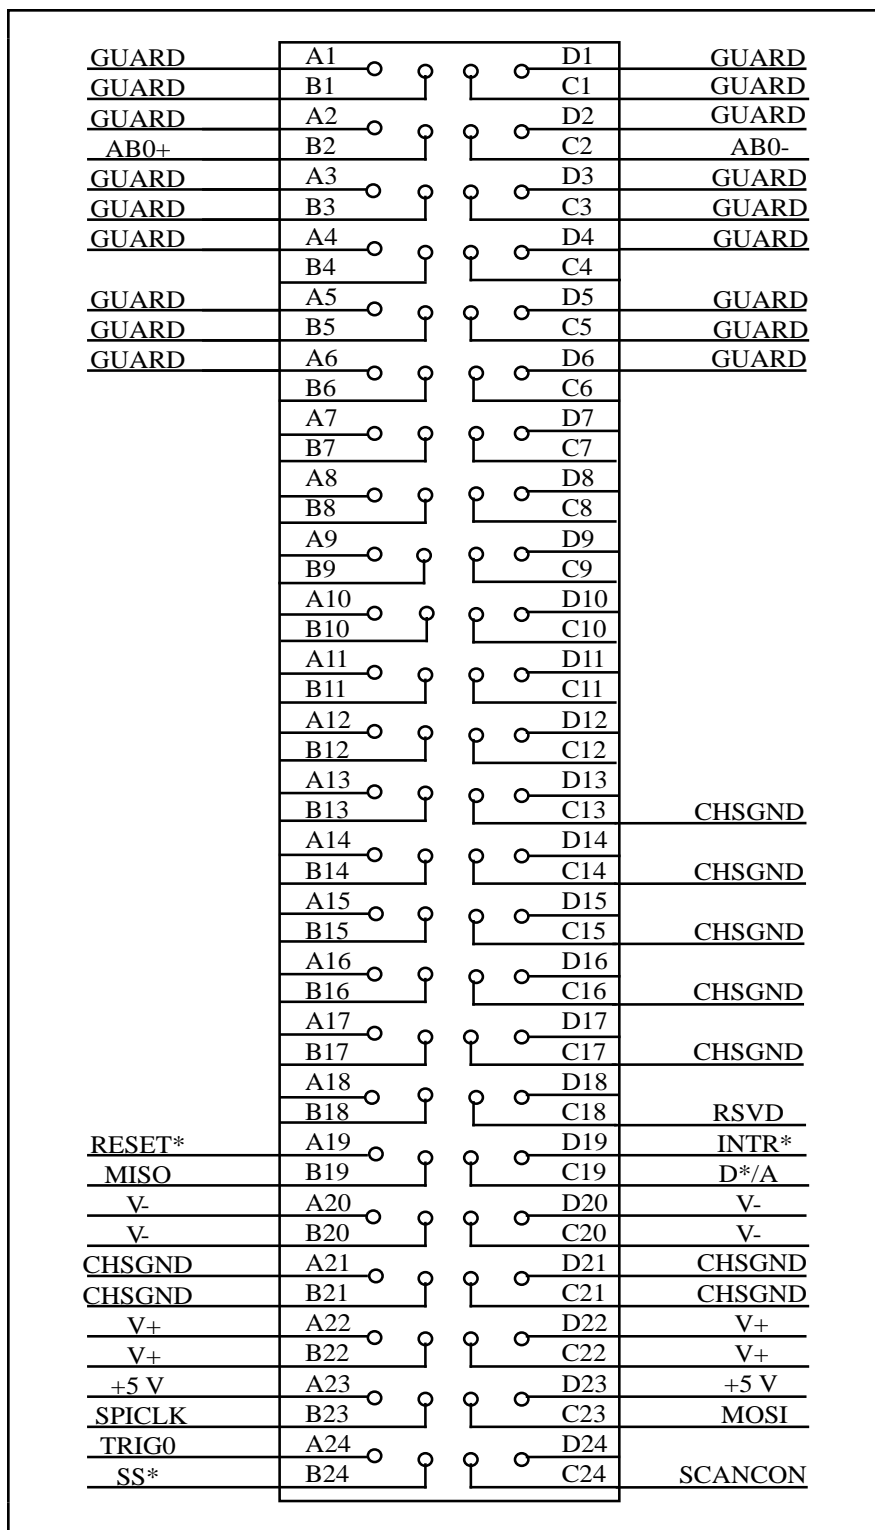


Figure 3-2. SCXIBus Connector Pin Assignment

SCXIBus Connector Signal Descriptions

Pin	Signal Name	Description
A1, B1, C1, D1, A2, D2, A3, B3, C3, D3, A4, D4, A5, B5, C5, D5, A6, D6	GUARD	Guard – Shields and guards the analog bus lines from noise.
B2	AB0+	Analog Bus 0+ – Positive analog bus 0 line. Used to multiplex several modules to one analog signal.
C2	AB0-	Analog Bus 0- – Negative analog bus 0 line. Used to multiplex several modules to one analog signal.
C13-C17, A21, B21, C21, D21	CHSGND	Chassis Ground – Digital and analog ground reference.
C18	RSVD	Reserved.
A19	RESET*	Reset – When pulled low, reinitializes the module to its power-up state. Totem pole. Input.
B19	MISO	Master-In Slave-Out – Transmits data from the module to the SCXIBus. Open collector. I/O.
C19	D*/A	Data/Address – Indicates to the module whether address information or data information is being sent to the module on MOSI. Open collector. I/O.
D19	INTR*	Interrupt – Active low. Causes data that is on MOSI to be written to the Slot-Select Register in Slot 0. Open collector. Output.
A20, B20, C20, D20	V-	Negative Analog Supply – -18.5 to -25 V.
A22, B22, C22, D22	V+	Positive Analog Supply – +18.5 to +25 V.
A23, D23	+5 V	+5 VDC Source – Digital power supply.
B23	SPICLK	Serial Peripheral Interface (SPI) Clock – Clocks the serial data on the MOSI and MISO lines. Open collector. I/O.
C23	MOSI	Master-Out Slave-In – Transmits data from the SCXIBus to the module. Open collector. I/O.

Pin	Signal Name	Description (continued)
A24	TRIG0	TRIG0 – General-purpose trigger line used by the SCXI-1121 to send SCANCLK to other modules or receive SCANCLK from other modules. Open collector. I/O.
B24	SS*	Slot Select – When low, enables module communications over the SCXIbus. Totem pole. Input.
C24	SCANCON	Scanning Control – Combination output enable and reload signal for scanning operations. Totem pole. Input.

All other pins are not connected.

MOSI, MISO, SPICLK, and SS* form a synchronous communication link that conforms with SPI using an idle-high clock and second-edge data latching. D*/A, INTR*, and RESET* are additional control signals.

When the module is being used in an SCXI-1000 or SCXI-1001 chassis, the data acquisition board, via the module rear signal connector, must tap into the open-collector backplane signal lines as a master to write to the module. The signal connections from the rear signal connector to the backplane are shown in Table 3-1.

Table 3-1. SCXIbus Equivalent for the Rear Signal Connector

Rear Signal Connector Signal	SCXIbus Equivalent
SERDATIN	MOSI
DAQD*/A	D*/A
SLOT0SEL*	INTR* Jumper W44 must be set to position 1
SERCLK	SPICLK
SERDATOUT	MISO Jumper W38 must be set to position 1

The SCXI-1121 module converts the data acquisition board signals to open-collector signals on the backplane of the SCXI chassis. In order for the data acquisition board to talk to a slot, the board must first assert the SS* for that slot. This is done by asserting INTR* low, writing a 16-bit number over MOSI corresponding to the desired slot (and chassis if an SCXI-1001 chassis is being used), and then releasing INTR* high. At this point, SS* of the desired slot is asserted low and the data acquisition board can communicate with the module in that slot according to the SPI protocol.

Digital Interface

Figure 3-3 shows a diagram of the SCXI-1121 and SCXIbus digital interface circuitry.

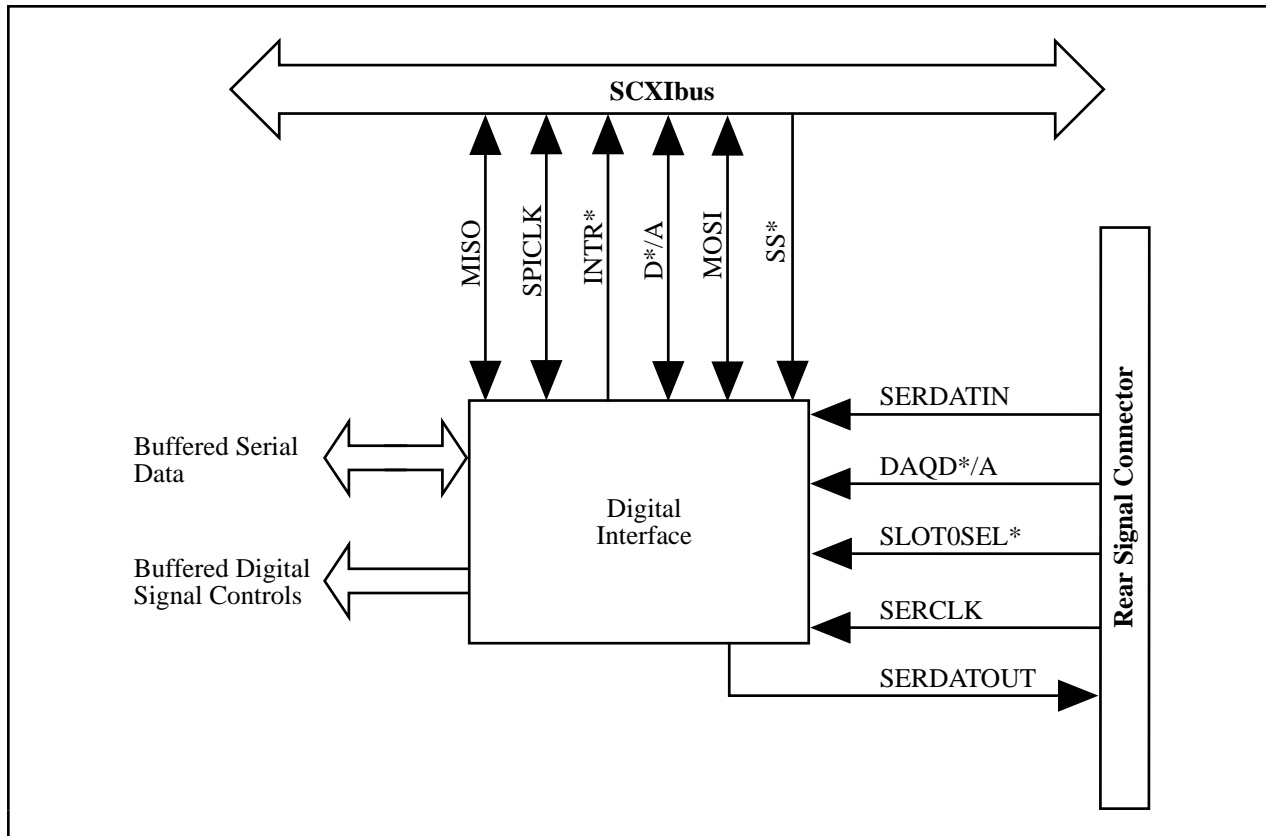


Figure 3-3. Digital Interface Circuitry Block Diagram

The digital interface circuitry is divided into a data acquisition section and an SCXIbus section. The SCXI-1121 connects to the SCXIbus via a 4x24 metal receptacle and to the data acquisition board via a 50-pin ribbon-cable header. The digital interface circuitry buffers the digital signals from the data acquisition board and from the SCXIbus and sends signals back and forth between the data acquisition board and the SCXIbus.

Digital Control Circuitry

Figure 3-4 diagrams the SCXI-1121 digital control.

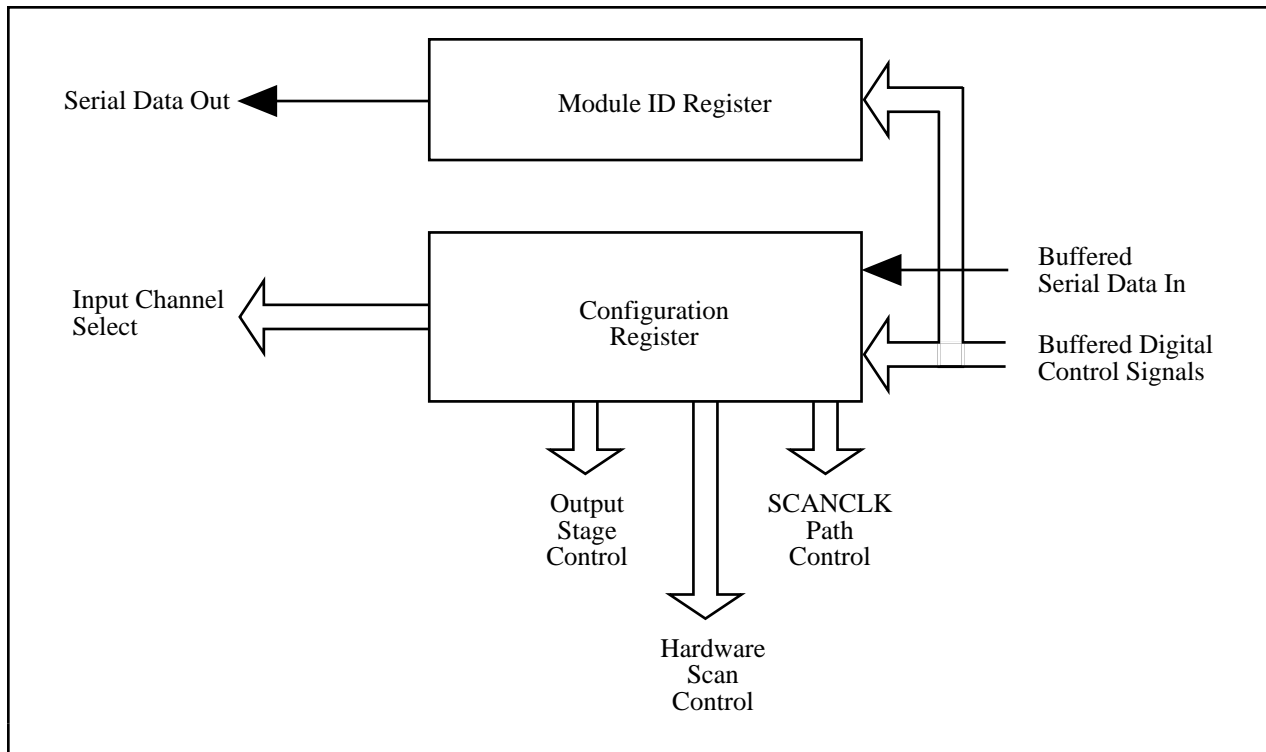


Figure 3-4. SCXI-1121 Digital Control

The digital control section consists of the Configuration Register and the Module ID Register.

The Configuration Register is a two-byte, serial-in parallel-out shift register. Data is received on the MOSI line from either Slot 0 or the data acquisition board when SS^* is enabled and D^*/A indicates data transfer (D^*/A low). The Configuration Register provides temperature channel selection and channel selection, and configures the SCXI-1121 for scanning options. All the control bits are fed into a latch before being routed to the rest of the module. The channel-select bits are taken directly from the shift register. Complete descriptions of the register bits are given in Chapter 4, *Register Descriptions*. Writes to the Configuration Register require the following steps:

1. SS^* goes low, enabling communication with the board.
2. D^*/A goes low, indicating that the information sent on the MOSI line is data.
3. The serial data is available on MOSI and $SPICLK$ clocks it into the register.
4. SS^* goes high and D^*/A goes high, indicating an end of communication. This action latches the Configuration Register bits.

When the SCXIBus is reset, all bits in the Configuration Register are cleared.

The Module ID Register connects to MISO on the SCXIbus. The Module ID Register is an 8-bit parallel/serial-in serial-out shift register and an SPI communication adapter. The contents of the Module ID Register are written onto MISO during the first four bytes of transfer after SS* has been asserted low. Zeros are written to MISO thereafter until SS* is released and reasserted. The SCXI-1121 module ID is hex 00000002.

Analog and Timing Circuitry

The SCXIbus provides analog power (± 18.5 VDC) that is regulated on the SCXI-1121 to ± 15 VDC, a guard, an analog bus (AB0 \pm), and a chassis ground (CHSGND). AB0 \pm buses the SCXI-1121 output to other modules or receives outputs from other modules via the SCXIbus. Refer to the *Calibration* section later in this chapter for more information. The guard guards the analog bus, and can be connected via jumper W33 to the analog ground reference or can be left floating (a connection can be made by another board).

The data acquisition board analog input and timing is the interface between the SCXI-1121 output and the data acquisition board. This is fully described in the following section.

Analog Input Channels

Figure 3-5 is a diagram of the analog input block.

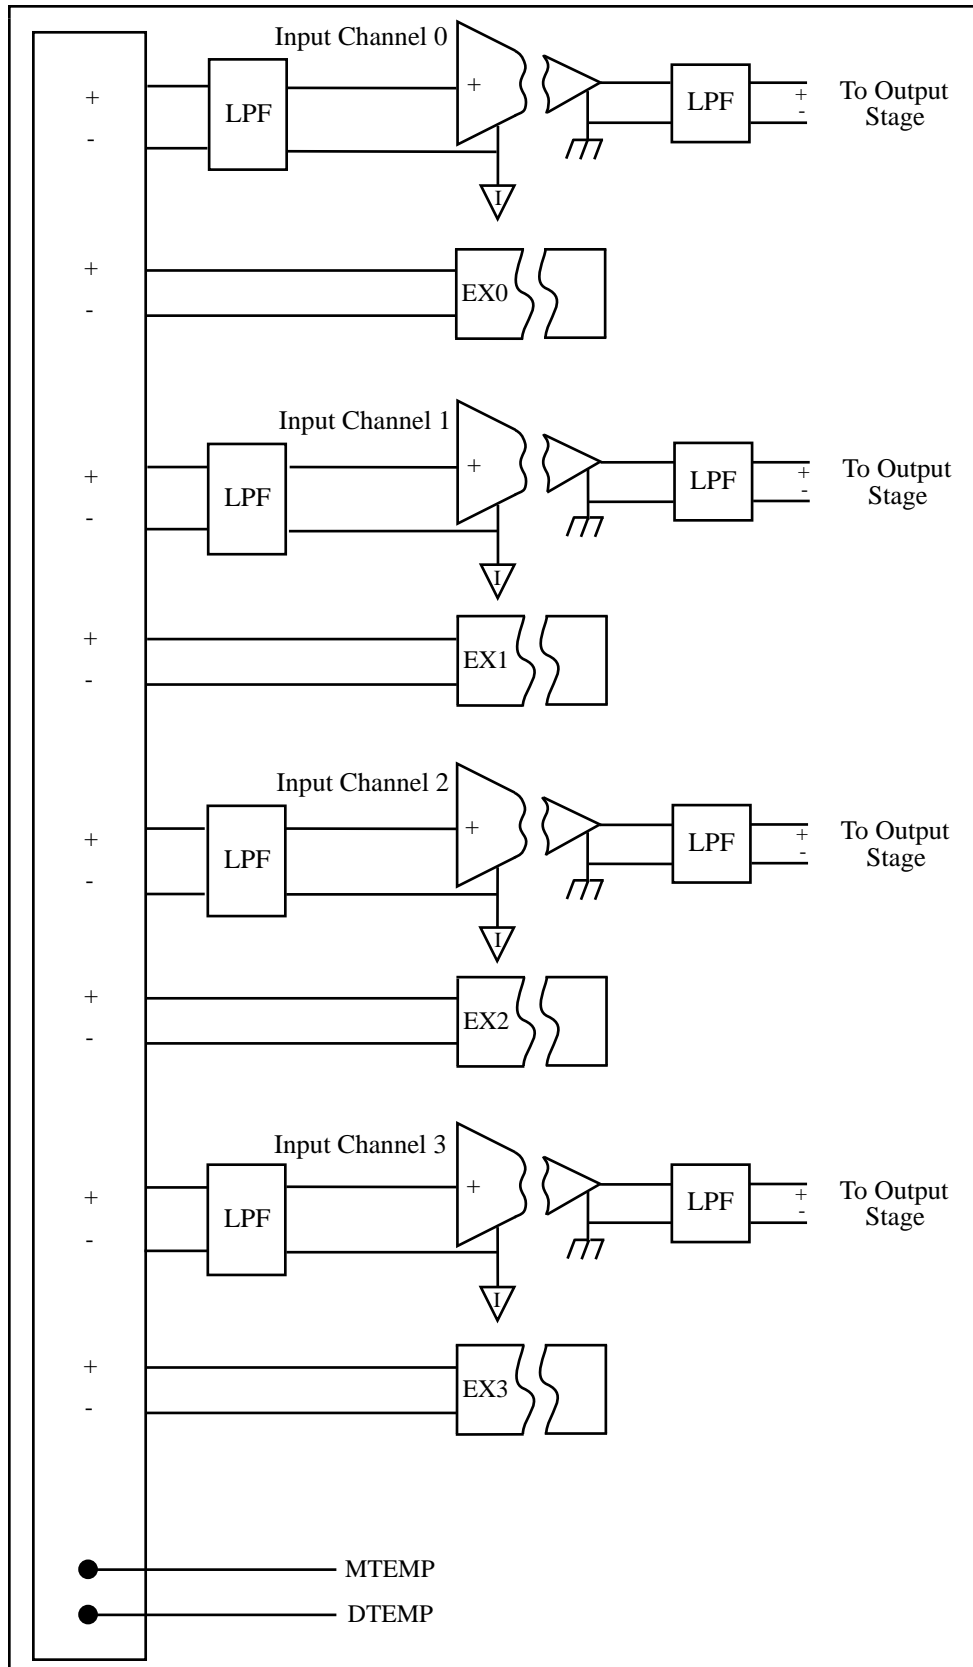


Figure 3-5. Analog Input Block Diagram

The analog input consists of four isolated single-ended noninverting amplifiers. In addition, lowpass filtering is available at the inputs. You can jumper select one of two bandwidths, 10 kHz or 4 Hz. The amplifier gain is divided into two stages, a first stage providing gains of 1, 10, 50, and 100, and a second stage providing gains of 1, 2, 5, 10, and 20. Also, the module has an internal completion network that can be used with half-bridge or quarter-bridge networks. Each channel is configurable to a different bandwidth, gain, or completion network operation.

Use the following formula to determine the overall gain of a given amplifier input channel:

$$G_{\text{total}} = G_{1\text{st}} \times G_{2\text{nd}}$$

where G_{total} is the overall gain and $G_{1\text{st}}$ and $G_{2\text{nd}}$ are the first and second-stage gains. It is important to note that the choice of gain in each stage will affect the amplifier bandwidth. To determine the bandwidth of a given gain stage use the following formula:

$$\text{BW} = \text{GBWP} / G$$

where BW is a given amplifier stage bandwidth, GBWP is the gain bandwidth product (typically 800 kHz), and G is the gain at this stage. This BW might be of concern at high first-stage gains such as 50 and 100. In this case the first-stage amplifier has a BW equal to 16 kHz and 8 kHz, respectively. Because of this decrease in the amplifier bandwidth, the channel overall bandwidth decreases, but noise immunity improves. If this bandwidth limitation is unacceptable, you should spread the gains over both stages, thus increasing the BW of each amplifier stage. In most cases this will introduce a negligible effect on the channel bandwidth. For example, to achieve a gain of 100, use $G_{1\text{st}} = 10$ and $G_{2\text{nd}} = 10$; for a gain of 1,000 use $G_{1\text{st}} = 50$ and $G_{2\text{nd}} = 20$.

All the amplifier input channels are overvoltage-protected to 240 Vrms with power on or off.

The isolated amplifiers fulfill two purposes on the SCXI-1121 module. They convert a small signal riding on a high common-mode voltage into a single-ended signal with respect to the SCXI-1121 chassis ground. With this conversion, the input analog signal can be extracted from a high common-mode voltage or noise before being sampled and converted by the data acquisition board. The isolated amplifier also amplifies and conditions an input signal, which results in an increase in measurement resolution and accuracy.

After isolation, further filtering is available to increase the noise immunity of the amplifier channel. It is important to note that the overall amplifier bandwidth is determined by both filtering stages, so to achieve the required bandwidth, both filtering sections should be set the same, as indicated in Chapter 2, *Configuration and Installation*.

Excitation Output Channels

In addition to the four input channels, the SCXI-1121 contains four fully isolated excitation channels, each corresponding to an input channel. For instance, input channel 0 corresponds to excitation channel 0. Each excitation channel consists of a voltage/current source with overvoltage protection and current limiting. Two levels of excitation are available for each mode of operation. In the voltage mode you can set the level to 3.333 V or 10 V; in the current mode you can set the level to 150 μA or 450 μA . You can choose one configuration out of the four available. To configure the excitation channels refer to Chapter 2, *Configuration and Installation*. The excitation channels are isolated from each other and are independently configurable for voltage or current excitation.

Calibration

Calibration Equipment Requirements

For best measurement results, calibrate the SCXI-1121 so that its offset is adjusted to 0 ± 3 mV RTO and 0 ± 6 μ V RTI and its excitation output is adjusted to $\pm 0.04\%$. According to standard practice, the equipment used to calibrate the SCXI-1121 should be 10 times as accurate as the SCXI-1121, that is, have 0.004% rated accuracy. Practically speaking, calibration equipment with four times the accuracy of the item under calibration is generally considered acceptable. Four times the SCXI-1121 accuracy is 0.016%. To calibrate the SCXI-1121 you need the following equipment.

- For the excitation channels, you need a voltmeter with the following specifications:
 - Accuracy: $\pm 0.004\%$ standard
 $\pm 0.016\%$ sufficient
 - Range: 0 to +5 V for 3.333 V and greater than + 10 V for 10 V
 - Resolution: 5 1/2 digits
- You also need a 120 Ω 1/4 W precision resistor with tempo less than or equal to 5 ppm, or an ammeter with the following specifications:
 - Accuracy: $\pm 0.004\%$ standard
 $\pm 0.016\%$ sufficient
 - Range: 0.5 mA
 - Resolution: 6 1/2 digits
- If you use the resistor to calibrate the current excitation, you also need an ohmmeter with four-wire measurement and the following specifications:
 - Accuracy: $\pm 0.004\%$ standard
 $\pm 0.016\%$ sufficient
 - Range: 200 Ω
 - Resolution: 5 1/2 digits

A multiranging 5 1/2-digit digital multimeter can provide you with most of the necessary functions described previously. We will refer to the measuring instrument as a digital multimeter (DMM).

Each channel on the SCXI-1121 has two potentiometers dedicated for calibration. For the amplifier channels, one potentiometer is used to null the output offset; the other is used to null the input offset. On the excitation channels, one potentiometer is used to adjust the voltage reference, while the other is used to adjust the current source.

Offset Null Adjust

Follow these steps to null the offset of the amplifier channels.

1. Short the inputs of the DMM together and then connect them to chassis ground.
2. Record the measurement indicated by the DMM display. This is the DMM inherent offset and should be subtracted from subsequent measurements.
3. Short the channel inputs of interest together and then to chassis ground.
4. Set the amplifier gain to 1.
5. Connect the amplifier output to the DMM. Make sure that the DMM can achieve the accuracy and resolution you need.
6. Adjust the output potentiometer of the channel of interest until the output is 0 ± 3 mV.
7. Set the amplifier gain to 1,000.
8. Adjust the input potentiometer of the channel of interest until the output is 0 ± 6 mV.
9. Go to the next channel.

To avoid erroneous results when nulling the amplifier, follow these steps in the order indicated.

Excitation Adjust

When calibrating the excitation channels, you should always start with the voltage excitation and then proceed to the current excitation, because the voltage excitation reference is used as a voltage reference for the current excitation. The following procedure will show you how to recalibrate your module excitation channel to the factory-calibration setting.

1. Connect a 120Ω precision resistor to the output of your excitation channel. Before connecting this resistor, measure it with a four-wire ohmmeter and record the exact value you have measured.
2. Set up the excitation channel of interest to 3.333 V excitation level.
3. Connect your DMM leads to the excitation output as close as possible to the resistor body.
4. Adjust the excitation voltage potentiometer until you read $3.333 \text{ V} \pm 0.04\%$.
5. Set up your channel for $150 \mu\text{A}$ excitation level.
6. Adjust the excitation current potentiometer until you read $(150 \mu\text{A} \times R_{120}) \text{ V} \pm 0.04\%$, where R_{120} is the measured value of the precision resistor.
7. Go to the next channel.

If you are using an ammeter to calibrate the current excitation level, you do not need a low-tempco resistor; a simple 120 Ω , 1%, 1/4 W, 100 ppm, metal-film resistor will do, and you do not need to measure the resistor. After following the previous procedure through step 4, follow these steps.

5. Remove the resistor from the excitation channel.
6. Set up your channel for 150 μA excitation level.
7. Connect the ammeter leads to the excitation channel output.
8. Adjust the excitation current potentiometer until you read 150 $\mu\text{A} \pm 0.04\%$.
9. Go to the next channel.

This procedure calibrates the 10 V and 450 μA levels at the same time but the accuracy achieved is limited to $\pm 0.2\%$. To achieve better accuracies at these levels, follow the procedure indicated above but set the excitation levels to 10 V and to 450 μA instead of 3.333 V and 150 μA . If you do so, the lower excitation levels of this channel will then be calibrated to $\pm 0.2\%$ instead of to 0.04%. In the factory, the module is calibrated for 3.333 V and 150 μA .

You can seal the potentiometers after calibration with antisabotage lacquer to avoid tampering with the calibration.

Table 3-2 lists the potentiometer reference designators that correspond to each channel.

Table 3-2. Calibration Potentiometer Reference Designators

Input Channel Number	Amplifier Channel		Excitation Channel	
	Input Null	Output Null	Voltage Mode	Current Mode
0	R2	R3	R10	R7
1	R16	R4	R20	R17
2	R26	R5	R30	R27
3	R36	R6	R40	R37

The resistor used to calibrate the current level must be a precision type with a tempco of 5 ppm or less. You should measure and record the resistor value before each calibration procedure. The DMM you are using should provide you with the required resolution and accuracy to achieve the calibration levels indicated in the paragraphs above. Annual or semi-annual calibration is recommended to maintain the accuracy level.

Analog Output Circuitry

Figure 3-6 shows the SCXI-1121 analog output circuitry.

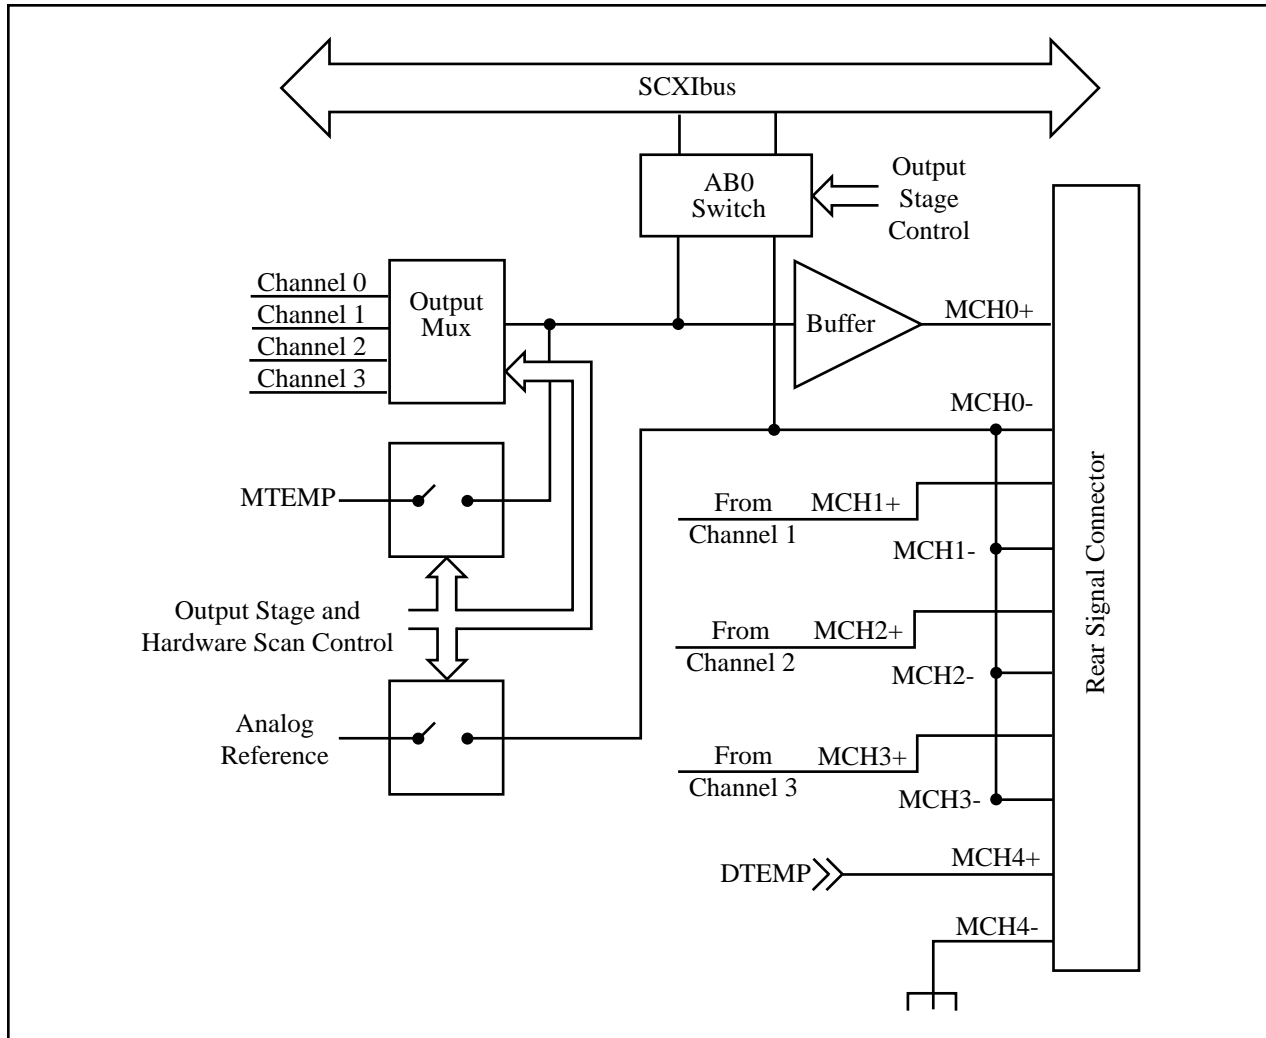


Figure 3-6. Analog Output Circuitry

The SCXI-1121 output circuitry consists of a buffered-output multiplexer and channel-select hardware. The channel-select hardware consists of a two-bit counter, MUXCOUNTER. This counter is needed when the board is operating in the Multiplexed-Output Mode. The counter output is sent to the multiplexer address pins to determine which of the four channels is to be connected to MCH0. In the Single-Channel Read mode, the MUXCOUNTER is loaded with the desired channel number. In the Scanning mode, the counter is loaded with the first channel to be read. During the scan, the counter is clocked by SCANCLK from the data acquisition board, or TRIG0 from the SCXibus, depending on the state of the CLKSELECT bit in the Configuration Register. During scanning operations, the MUXCOUNTER is reloaded with the channel value stored in the Configuration Register when SCANCON is high (inactive) and will count upwards on each rising clock edge when SCANCON is low (active). In the Parallel-Output Mode, the MUXCOUNTER is disabled and its output indicates binary 00; hence, amplifier channel 0 is

selected at the output multiplexer and is connected to MCH0. The three other channels are hardwired to MCH1 through MCH3 on the rear signal connector.

The output multiplexer multiplexes all four amplifier outputs and the temperature sensor reading provided on the MTEMP line. To read the temperature sensor when it is multiplexed with the other input channels, set the RTEMP bit of the Configuration Register high. This measurement is only software controlled. For hardware control of the temperature sensor reading, connect the temperature sensor to MCH4+. Notice that MCH4-, the DTS reference, is hardwired to the chassis ground. The multiplexer output connects to the MCH0± and is connected to the data acquisition board analog channel input. In the case of the MIO data acquisition boards, MCH0± on the rear signal connector corresponds to ACH0 and ACH8.

Furthermore, you can bus the multiplexed output of the SCXI-1121 via switches to AB0± on the SCXIbus and on to other modules. When you use multiple modules, you can bus the output of the module via AB0 to the module that is connected to the data acquisition board. In this case, the AB0 switches of all the modules are closed, whereas the output multiplexer of all the modules but the one being read are disabled. Refer to chapters 2 and 5 for further details on how to configure and program multiple modules.

In addition to the Multiplexed-Output mode described in the previous paragraph, you can operate the SCXI-1121 in Parallel-Output mode. In this mode, you need no software—other than software used with your data acquisition board—to control the scanning of the four channels or to perform a single read. To access the temperature sensor in this mode, configure the temperature sensor in the DTS mode. At power up or at reset, amplifier channel 0 is selected on the output multiplexer, and hence connects to MCH0. The other four channels (three amplifier channels and one temperature channel) are hardwired to the rear signal connector. Notice that even when you select the Multiplexed-Output mode, the SCXI-1121 drives the rear signal connector pins 5 through 12. The SCXI-1121 outputs on the rear signal connector are short-circuit protected.

Refer to the following *Scanning Modes* section for further details on how to scan the SCXI-1121 channels.

Scanning Modes

There are four basic types of scanning modes possible with the SCXI-1121—single-module parallel scanning, single-module multiplexed scanning, multiple-module multiplexed scanning, and multiple-chassis scanning (possible only with the SCXI-1001 chassis). For additional information, consult Chapter 2, *Configuration and Installation*, Chapter 5, *Programming*, your data acquisition board manual, and your SCXI chassis user manual. If you need further information, contact National Instruments.

Single-Module Parallel Scanning

Single-Module parallel scanning is the simplest scanning mode. Directly cable the SCXI-1121 to the data acquisition board as shown in Figure 3-7. In this configuration, each analog signal has its own channel. Timing signals are not necessary for this type of scanning because the module provides all channels to the data acquisition board at all times. You can implement single-module parallel scanning with any data acquisition board that is appropriately cabled to the SCXI-1121.

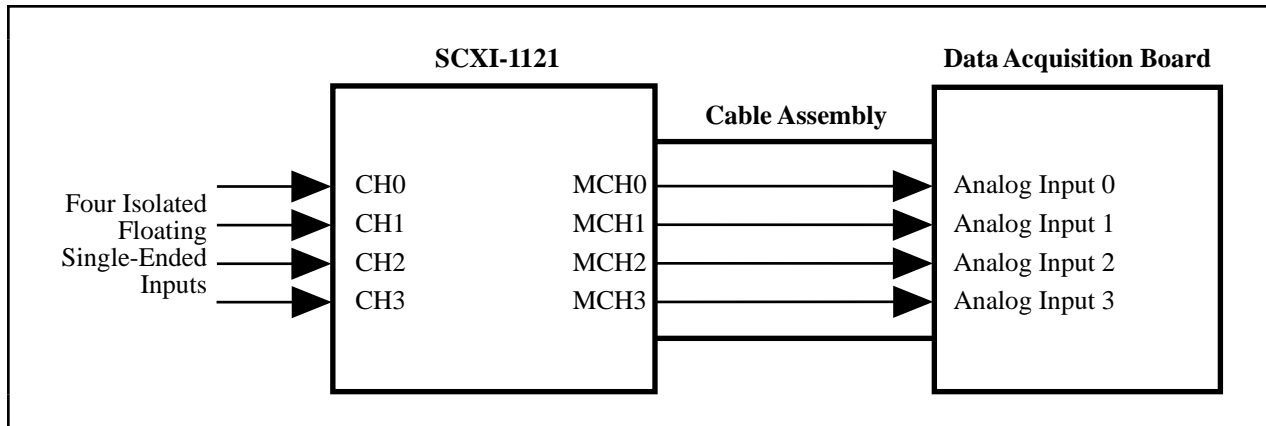


Figure 3-7. Single-Module Parallel Scanning

Multiplexed Scanning

Only the MIO-16 data acquisition boards support multiplexed scanning on the SCXI-1121. During multiplexed scanning, a module sends the SCANCLK signal to Slot 0 over the TRIG0 backplane line, and Slot 0 sends unique SCANCON signals to each module. Each module uses its signal to reload MUXCOUNTER and to determine when the SCXI-1121 output is enabled. Slot 0 contains a module list first-in-first-out (FIFO) memory chip, similar to the Channel/Gain FIFO on an MIO-16 board, except that instead of having a channel number and gain setting for each entry, the Slot 0 FIFO contains a slot number and a sample count for each entry. The list in Slot 0 will determine which module is being accessed and for how many samples. It is important that you make sure that the lists on the data acquisition board and Slot 0 are compatible so that the samples are acquired as intended. See your SCXI chassis manual for more information.

Single-Module Multiplexed Scanning

Single-Module Multiplexed Scanning (Direct)

This is the simplest multiplexed scanning mode. Directly cable the SCXI-1121 to the data acquisition board as shown in Figure 3-8. The module sends SCANCLK onto TRIG0, and Slot 0 sends SCANCON back to the module. SCANCON will be low at all times during the scan except during changes from one Slot 0 scan list entry to the next, when SCANCON pulses high to make the MUXCOUNTER reload its starting channel. Notice that although you are using only a single module, you can put many entries with different counts in the Slot 0 FIFO, so that some channels are read more often than others. You cannot change the start channel in the module Configuration Register during a scan.

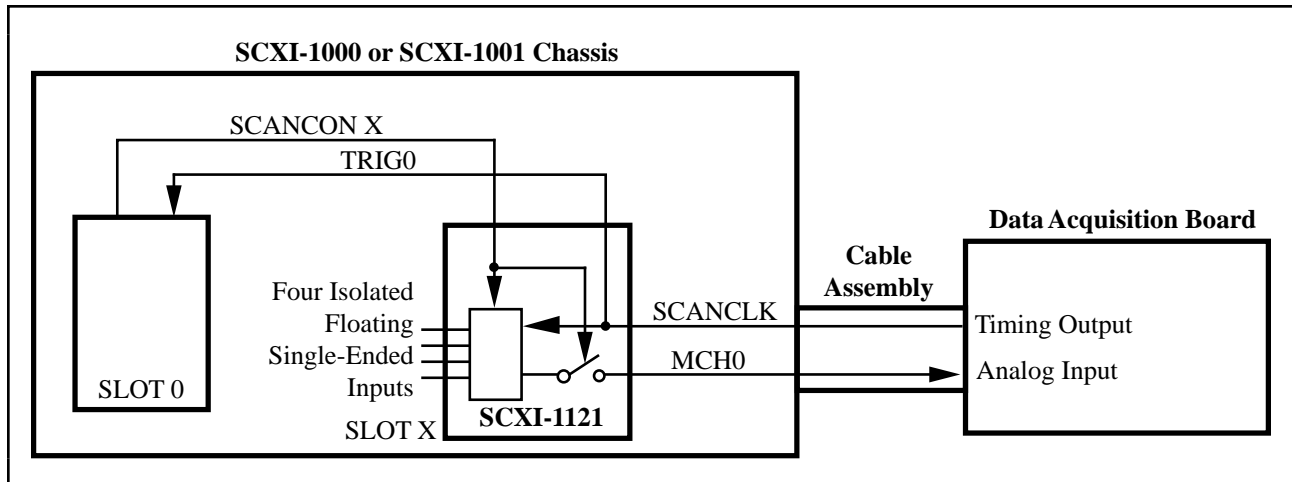


Figure 3-8. Single-Module Multiplexed Scanning (Direct)

Single-Module Multiplexed Scanning (Indirect)

In this mode, the SCXI-1121 is not directly cabled to the data acquisition board. Instead, you connect another module to the data acquisition board, and the analog output of the SCXI-1121 is sent over Analog Bus 0, through the intermediate module, and then to the data acquisition board. The SCXI-1121 receives its MUXCOUNTER clock from TRIG0, which is sent by the intermediate module, as illustrated in Figure 3-9. Slot 0 operation is the same for direct connection scanning.

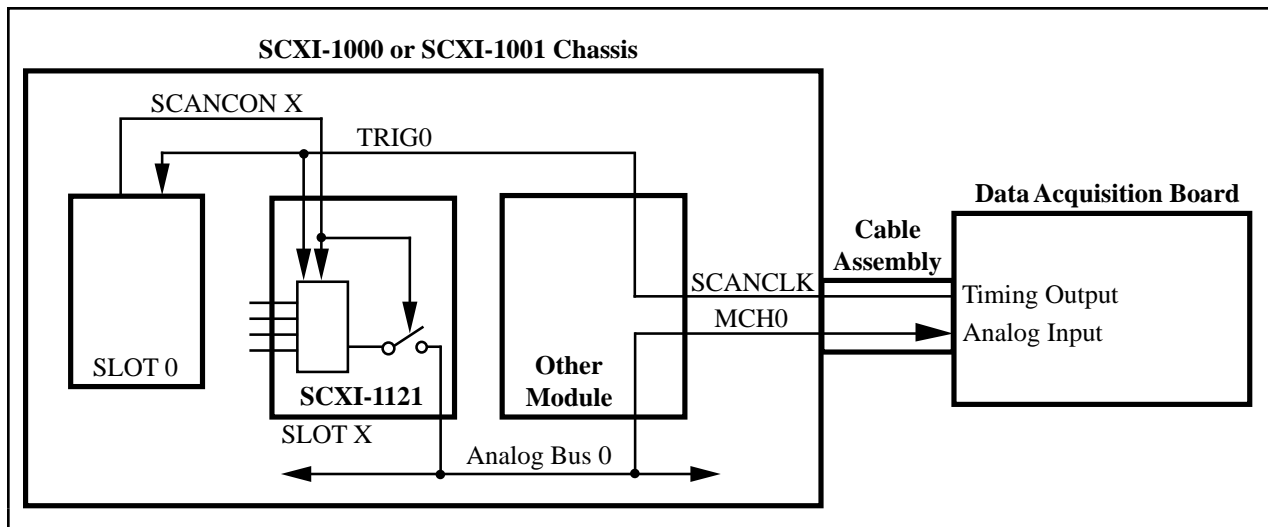


Figure 3-9. Single-Module Multiplexed Scanning (Indirect)

Multiple-Module Multiplexed Scanning

In this mode, all the modules tie into Analog Bus 0, and SCANCON enables the output of their amplifiers. The module that is directly cabled to the data acquisition board sends SCANCLK onto TRIG0 for the other modules and Slot 0, as illustrated in Figure 3-10. The scan list in Slot 0 is programmed with the sequence of modules and the number of samples per entry.

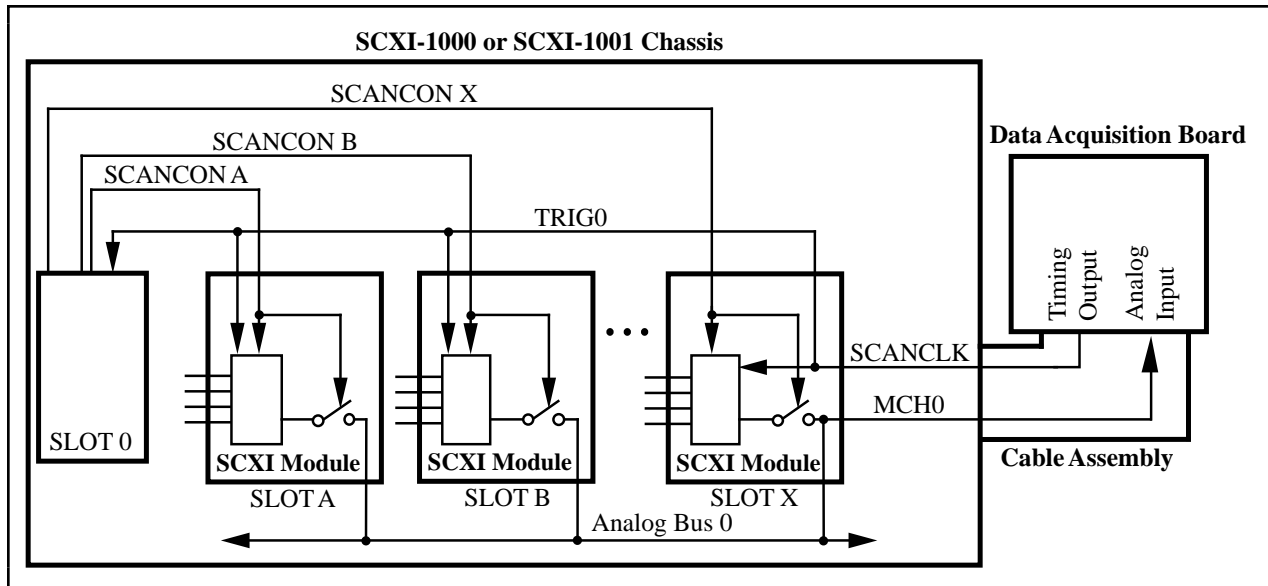


Figure 3-10. Multiple-Module Multiplexed Scanning

Multiple-Chassis Scanning

In this mode, you attach each SCXI-1001 chassis to a daisy chain of cable assemblies and multichassis adapter boards, as illustrated in Figure 3-11. You program each chassis separately, and each chassis occupies a dedicated channel of the data acquisition board. Within each chassis, scanning operations act as if the other chassis are not being used, with one exception. You must program the Slot 0 scan list in each chassis with dummy entries of Slot 13 to fill the samples when the data acquisition board will be sampling another chassis or data acquisition board channel. This will keep the chassis synchronized. Notice that you can only perform multiple-chassis scanning with the SCXI-1001 chassis and MIO-16 data acquisition boards. See Chapter 5, *Programming*, for more information on multiple-chassis scanning. See Appendix E, *SCXI-1121 Cabling*, for more information on the necessary cable accessories for multichassis scanning.

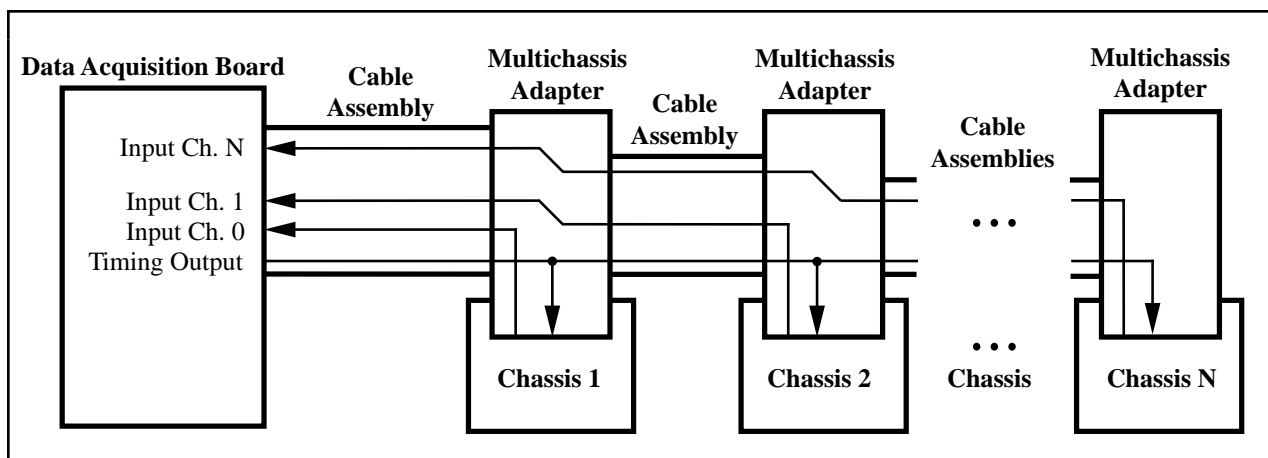


Figure 3-11. Multiple-Chassis Scanning

Chapter 4

Register Descriptions

This chapter describes in detail the SCXI-1121 Module ID Register, the Configuration Register, the Slot 0 registers, and multiplexer addressing.

Note: If you plan to use a programming software package such as NI-DAQ, LabWindows, or LabVIEW with your SCXI-1121 board, you do not need to read this chapter.

Register Description

Register Description Format

The register description chapter discusses each of the SCXI-1121 registers and the Slot 0 registers. A detailed bit description of each register is given. The individual register description gives the type, word size, and bit map of the register, followed by a description of each bit.

The register bit map shows a diagram of the register with the MSB shown on the left (bit 15 for a 16-bit register, bit 7 for an 8-bit register), and the LSB shown on the right (bit 0). A rectangle is used to represent each bit. Each bit is labeled with a name inside its rectangle. An asterisk (*) after the bit name indicates that the bit is inverted (negative logic). The Module ID register has a unique format described in the *Module ID Register* section.

In many of the registers, several bits are labeled with an X, indicating *don't care* bits. When you write to a register you may set or clear these bits without effect.

SCXI-1121 Registers

The SCXI-1121 has two registers. The Module ID Register is a four-byte, read-only register that contains the Module ID number of the SCXI-1121. The Configuration Register is a 16-bit, write-only register that controls the functions and characteristics of the SCXI-1121.

Module ID Register

The Module ID Register contains the 4-byte module ID code for the SCXI-1121. This code number will be read as the first four bytes on the MISO line whenever the module is accessed. The bytes will appear least significant byte first. Within each byte, data is sent out most significant bit first. Additional data transfers will result in all zeros being sent on the MISO line. The Module ID Register is reinitialized to its original value each time the SCXI-1121 is deselected by the SS* signal on the backplane.

Type: Read-only

Word Size: 4-byte

Bit Map:

Byte 0

7	6	5	4	3	2	1	0
0	0	0	0	0	0	1	0

Byte 1

7	6	5	4	3	2	1	0
0	0	0	0	0	0	0	0

Byte 2

7	6	5	4	3	2	1	0
0	0	0	0	0	0	0	0

Byte 3

7	6	5	4	3	2	1	0
0	0	0	0	0	0	0	0

Configuration Register

The Configuration Register contains 16 bits that control the functions of the SCXI-1121. When SS* is asserted (low) and D*/A indicates data (low), the register will shift in the data present on the MOSI line, bit 15 first, and then latch it when the SCXI-1121 is deselected by the SS* signal on the backplane. The Configuration Register initializes to all zeros when the SCXI chassis is reset or first turned on.

Type: Write-only

Word Size: 16-bit

Bit Map:

15	14	13	12	11	10	9	8
CLKOUTEN	CLKSELECT	SCAL	X	X	X	CHAN1	CHAN0
7	6	5	4	3	2	1	0
X	X	RTEMP	RSVD	SCANCLKEN	SCANCONEN	ABOEN	FOUTEN*

Bit	Name	Description
15	CLKOUTEN	Scanlock Output Enable – This bit determines whether the SCANCLK signal from the rear signal connector is sent out, in inverted form, to the TRIG0 backplane signal. If CLKOUTEN is set to 1, SCANCLK* is transmitted on TRIG0. If CLKOUTEN is cleared to 0, SCANCLK* is not transmitted on TRIG0.
14	CLKSELECT	Scanlock Select – This bit determines whether the SCXI-1121 uses SCANCLK or the inverted form of TRIG0 to clock the MUXCOUNTER for the purpose of scanning through the analog channels. If CLKSELECT is cleared to 0, SCANCLK is used to clock MUXCOUNTER. If CLKSELECT is set to 1, TRIG0* is used as the source to clock MUXCOUNTER.
13	SCAL	Shunt Calibrate – This bit determines whether the shunt calibration switches on the SCXI-1321 are closed or open. If SCAL is cleared to 0, the switches are open. If SCAL is set to 1, the shunt calibration switches on the SCXI-1321 are closed and an R _{SCAL} is placed in parallel with the bridge between EX+ and CH+ on all four channels.
12-10, 7-6	X	Don't care bits.
9-8	CHAN<1..0>	Channel Select – These bits determine the channel number (zero to three) that is loaded into the MUXCOUNTER to determine the analog channel to be read during a single read, or the starting channel on the module for a scanned data acquisition. CHAN1 is the MSB.

Bit	Name	Description (continued)
5	RTEMP	Read Temperature – This bit determines whether the selected channel output or the MTEMP signal is driven onto the MCH0± pins of the rear signal connector. If RTEMP is cleared to zero, the selected channel output is used as the module output. If RTEMP is set to one, the MTEMP signal is used as the module output. The module output will only be driven when FOUTEN* is cleared to 0, or SCANCON is active (low) while SCANCONEN* is cleared.
4	RSVD	Reserved – This bit should always be written to zero.
3	SCANCLKEN	Scan Clock Enable – This bit determines whether MUXCOUNTER will increment on each clock signal (the clock source is determined by CLKSELECT), or keep its loaded value. If SCANCLKEN is set to one, MUXCOUNTER will be clocked during scans. If SCANCLKEN is cleared to zero, MUXCOUNTER will not be clocked.
2	SCANCONEN	Scan Control Enable – This bit, when high, enables the SCANCON signal.
1	AB0EN	Analog Bus 0 Enable – This bit determines whether Analog Bus 0 on the SCXIbus drives MCH0 on the rear signal connector. If AB0EN is cleared to zero, Analog Bus 0 does not drive MCH0. If AB0EN is set to one, Analog Bus 0 + drives MCH0+ through a buffer and a Analog Bus 0 - is connected to MCH0-.
0	FOUTEN*	Forced Output Enable – This bit determines whether the module will drive the MCH0± pins on the rear signal connector with either the selected channel output or the MTEMP signal, depending on the state of RTEMP. If FOUTEN* is cleared to zero, the MCH0± pins will be driven through a buffer by the selected channel output or the MTEMP line. If FOUTEN* is set to one, the MCH0± pins will not be driven by the selected channel output or MTEMP, unless SCANCON is active (low) and the SCANCONEN bit is cleared. If the selected channel output or MTEMP is driving the output buffer, it will drive Analog Bus 0 if AB0EN is set. If nothing is driving the output buffer, the SCXI-1121 output will saturate.

Slot 0 Register Descriptions

Slot 0 has three registers. The Slot-Select Register is a 16-bit, write-only register that determines with which slot the data acquisition board will speak when SLOT0SEL* is released high. In the case of the SCXI-1001 chassis, the Slot-Select Register also determines in which chassis the desired slot is. The FIFO Register is a 16-bit, write-only register used for storing the Slot 0 scan list that determines the chassis scan sequence. The Hardscan Control Register (HSCR) is an 8-bit, write-only register used for setting up the timing circuitry in Slot 0. The Slot-Select Register is written to by using the SLOT0SEL* line. The HSCR and the FIFO Register are written to as if they were registers located on modules in Slots 13 and 14. It is recommended that you maintain software copies of the Slot-Select Register, HSCRs, and all the Slot 0 scan lists that correspond to the writes to FIFO Registers.

If you are using multiple chassis, it is important to understand the architectural differences of the Slot-Select Register as compared to the HSCR and the FIFO Register. Although each chassis has its own physical Slot-Select Register, all are written to at the same time. The jumper settings in Slot 0 of a chassis determine with which chassis number Slot 0 is identified. From the software perspective, only one Slot-Select Register exists in a system composed of multiple chassis. The HSCR and FIFO Register, on the other hand, are unique to each chassis and you must program them separately.

Slot-Select Register

The Slot-Select Register contains 16 bits that determine which module in which chassis will be enabled for communication when the SLOTOSEL* line is set to one. An SCXI-1000 chassis will select the appropriate module in its chassis, regardless of the chassis number written. The Slot-Select Register will shift in the data present on the MOSI line, bit 16 first, when SLOTOSEL* is cleared to zero.

Type: Write-only

Word Size: 16-bit

Bit Map:

15	14	13	12	11	10	9	8
X	X	X	X	X	X	X	CHS4
7	6	5	4	3	2	1	0
CHS3	CHS2	CHS1	CHS0	SL3	SL2	SL1	SL0

Bit	Name	Description
15-9	X	Don't care bits.
8-4	CHS<4..0>	Chassis Bit 4 through 0 – These bits determine which chassis is selected. On the SCXI-1000 chassis, these bits are don't cares.
3-0	SL<3..0>	Slot Bit 3 through 0 – These bits determine which slot in the selected chassis is selected.

Hardscan Control Register (HSCR)

The HSCR contains eight bits that control the setup and operation of the hardscan timing circuitry of Slot 0. To write to the HSCR, follow the procedure given in the *Register Writes* section of Chapter 5, *Programming*, using 13 as the slot number, and writing eight bits to the HSCR. The register will shift in the data present on the MOSI line, bit seven first, when Slot 13 is selected by the Slot-Select Register.

Type: Write-only

Word Size: 8-bit

Bit Map:

7	6	5	4	3	2	1	0
RSVD	FRT	RD	ONCE	HSRS*	LOAD*	SCANCONEN	CLKEN

Bit	Name	Description
7	RSVD	Reserved.
6	FRT	Forced Retransmit – This bit, when clear, causes the scan list in the FIFO to be reinitialized to the first entry, thus allowing the scan list to be reprogrammed in two steps instead of having to rewrite the entire list. When this bit is set, it has no effect.
5	RD	Read – This bit, when clear, prevents the FIFO from being read. When set, the FIFO is being read except at the end of a scan list entry during scanning, when reading is briefly disabled to advance to the next scan list entry.
4	ONCE	Once – When set, this bit will cause the Hardscan circuitry to shut down at the end of the scan list circuitry during a data acquisition. When clear, the circuitry will wrap around and continue with the first scan list entry after the entry is finished.
3	HSRS*	Hardscan Reset – When clear, this bit causes all the hardware scanning circuitry, including the FIFO, to be reset to the power up state. When set, this bit has no effect.
2	LOAD*	Load – This bit, when clear, forces a loading of the Slot 0 sample counter with the output of the FIFO. When set, this bit has no effect.
1	SCANCONEN	Scan Control Enable – When set, this bit enables the SCANCON lines. When clear, all SCANCON lines are disabled (high).
0	CLKEN	Clock Enable – When set, this bit enables TRIG0 as a clock for the hardscan circuitry. When clear, TRIG0 is disabled.

FIFO Register

The FIFO Register is used to add entries to the Slot 0 FIFO. The FIFO contains the Slot 0 scan list. Each entry contains a slot number to be accessed, and a count number to determine the number of samples to be taken from that slot. To write to the FIFO Register, follow the procedure given in the *Register Writes* section of Chapter 5, *Programming*, using 14 as the slot number, and writing 16 bits to the FIFO Register. The register will shift in the data present on the MOSI line, bit 15 first, when Slot 14 is selected by the Slot-Select Register. The Slot 0 scan list is created by consecutive writes to the FIFO Register. Each write creates a new entry at the end of the scan list. The maximum number of entries is 256. To clear the FIFO of all entries, clear the HSRs* bit in the HSCR.

Type: Write-only

Word Size: 16-bit

Bit Map:

15	14	13	12	11	10	9	8
X	X	X	X	X	MOD3	MOD2	MOD1
7	6	5	4	3	2	1	0
MOD0	CNT6	CNT5	CNT4	CNT3	CNT2	CNT1	CNT0

Bit	Name	Description
15-11	X	Don't care bits – Unused.
10-7	MOD<3..0>	Module Number – The value of these bits plus one determines the number of the slot to be accessed for this scan entry. For example, to access Slot 6, MOD<3..0> would be 0101.
6-0	CNT<6..0>	Count – The value of these bits plus one determines how many samples will be taken before the next scan list entry becomes active. A value of zero corresponds to one sample and a value of 127 corresponds to 128 samples.

Chapter 5

Programming

This chapter contains a functional programming description of the SCXI-1121 and Slot 0.

Note: If you plan to use a programming software package such as NI-DAQ, LabWindows, or LabVIEW with your SCXI-1121 board, you do not need to read this chapter.

Programming Considerations

Programming the SCXI-1121 involves writing to the Configuration Register. Programming Slot 0 involves writing to the HSCR and FIFO Register. Programming the data acquisition boards involves writes to their registers. See your data acquisition board user manual for more information. The programming instructions list the sequence of steps to take. The instructions are language independent; that is, they instruct you to write a value to a given register without presenting the actual code.

Notation

For the bit patterns to be written, the following symbols are used:

- 0 Binary zero
- 1 Binary one
- X Don't care, either zero or one may be written
- C One of two bits used to specify the channel to be loaded into the MUXCOUNTER. This value will either be the channel to be read for single reads, or a starting channel for scanned measurements.

The 16-bit patterns are presented MSB first, left to right.

Register Writes

This section describes how to write to the Configuration Register, HSCR, and FIFO Register including the procedure for writing to the Slot-Select Register to select the appropriate slot. For timing specifics, refer to the *Timing Requirements and Communication Protocol* section in Chapter 2, *Configuration and Installation*. The rear signal connector pin equivalences to the different National Instruments data acquisition boards are given in Table 4-1. See also Appendix E, *SCXI-1121 Cabling*. The Configuration Register, the FIFO Register, and the HSCR are write-only registers.

The different bits in these registers often control independent pieces of circuitry. There are times when you may want to set or clear a specific bit or bits without affecting the remaining bits. However, a write to one of these registers will affect all bits simultaneously. You cannot read the registers to determine which bits have been set or cleared in the past; therefore, you should maintain a software copy of these registers. You can then read the software copy to determine the status of the register. To change the state of a single bit without disturbing the remaining bits, set or clear the bit in the software copy and write the software copy to the register.

Table 5-1. SCXI-1121 Rear Signal Connector Pin Equivalences

SCXIBus Line	SCXI-1121 Rear Signal Connector	MIO-16	Lab Board	PC-LPM-16
MOSI D*/A INTR* SPICLK MISO	SERDATIN DAQD*/A SLOT0SEL* SERCLK SERDATOUT	ADIO0 ADIO1 ADIO2 EXTSTROBE* BDIO0	PB4 PB5 PB6 PB7 PC1	DOUT4 DOUT5 DOUT6 DOUT7 DIN6

Register Selection and Write Procedure

1. Select the slot of the module to be written to (or Slot 13 or 14). Initial conditions:
 - SERDATIN = X
 - DAQD*/A = X
 - SLOT0SEL* = 1
 - SERCLK = 1
2. Clear SLOT0SEL* to 0. This will deassert all SS* lines to all modules in all chassis.
3. For each bit, starting with the MSB first (bit 15):
 - a. SERDATIN = bit to be sent. These bits are the data that is being written to the Slot-Select Register.
 - b. Clear SERCLK to 0.
 - c. Set SERCLK to 1. This rising edge clocks the data. (If you are using an MIO-16 board, writing to the EXTSTROBE* register will pulse EXTSTROBE* low and then high, accomplishing steps 3b and 3c.)
4. Set SLOT0SEL* to 1. This will assert the SS* line of the module whose slot number was written to Slot 0. If you are using multiple chassis, the appropriate slot in the chassis whose address corresponds to the written chassis number will be selected automatically. When no communications are taking place between the data acquisition board and any modules, write zero to the Slot-Select Register to ensure that no accidental writes occur.
5. If you are writing to a Configuration Register, clear DAQD*/A to 0 (this indicates data will be written to the Configuration Register). If you are writing to the HSCR or FIFO Register, leave DAQD*/A high.
6. For each bit to be written to the Configuration Register:
 - a. Establish the desired SERDATIN level corresponding to this bit.
 - b. Clear SERCLK to 0.
 - c. Set SERCLK to 1 (clock the data). (If you are using an MIO-16 board, writing to the EXTSTROBE* register will pulse EXTSTROBE* low and then high, accomplishing steps 6b and 6c.)

7. Pull SLOT0SEL* low to deassert the SS* line, latch the data into the Configuration Register and establish conditions for writing a new slot select number to the Slot 0 Slot-Select Register.
8. If you are not selecting another slot, write zero to the Slot 0 Slot-Select Register. If you are selecting another slot, start at step 3.

For a timing illustration of a Configuration Register write, see Figure 2-18, *Configuration Register Write Timing Diagram*, which shows the proper write to configure an SCXI-1121 that is directly cabled to an MIO-16 for multiple-module multiplexed scanning with a start channel of 3.

Initialization

The SCXI-1121 powers up with its Configuration register cleared to all zeros. You can force this state by an active low signal on the RESET* pin of the backplane connector. In the reset state, CH0 through CH3 are routed to MCH0 through MCH3 on the rear signal connector. The module is disconnected from Analog Bus 0 and disabled from scanning.

Single-Channel Measurements

This section describes how to program the SCXI-1121, either alone or in conjunction with other modules, to make single-channel, or non-scanned, measurements.

Direct Measurements

Parallel Output

In order to perform a parallel output measurement, you must cable the SCXI-1121 rear signal connector to a data acquisition board with each output connected to a different data acquisition board channel. See Chapter 2, *Configuration and Installation*, for more information. For information on how to make the voltage measurement with your data acquisition board, consult your data acquisition board user manual. Remember to account for the gains of both the SCXI-1121 and the data acquisition board when calculating the actual voltage present at the input of the SCXI-1121.

To measure one of the four differential input channels to the SCXI-1121, or the DTEMP line if the module has been configured appropriately, perform the following steps:

1. Write the binary pattern 000XXX00 XX000000 to the SCXI-1121 Configuration Register. Notice that this can be the RESET state.
2. Measure the voltage with the data acquisition board.

Multiplexed Output

In order to perform a direct multiplexed output measurement, you must cable the SCXI-1121 rear signal connector to a data acquisition board. See Chapter 2, *Configuration and Installation*, for more information. For information on how to make the voltage measurement with your data acquisition board, consult your data acquisition board user manual. Remember to account for the

gains of both the SCXI-1121 and the data acquisition board when calculating the actual voltage present at the input of the SCXI-1121.

To measure one of the four differential input channels to the SCXI-1121, perform the following steps:

1. Write the binary pattern `000XXXCC XX000000` to the SCXI-1121 Configuration Register.
2. Measure the voltage with the data acquisition board.

To shunt calibrate one of the four differential input channels, perform the following steps:

1. Write the binary pattern `001XXXCC XX000000` to the SCXI-1121 Configuration Register. Insert a delay of at least 1 sec if you have set the 4 Hz filter, or at least 1 msec if you have set the 10 kHz filter. This delay permits the SCXI-1121 amplifier to settle.
2. Measure the voltage with the data acquisition board.

To measure the voltage on the MTEMP line, perform the following steps:

1. Write the binary pattern `000XXXXX XX100000` to the SCXI-1121 Configuration Register.
2. Measure the voltage with the data acquisition board.

Indirect Measurements

Indirect measurements involve one module sending a signal to Analog Bus 0, where it is picked up by another module and transmitted to the data acquisition board.

Measurements from Other Modules

To perform measurements from other modules, you must cable the SCXI-1121 rear signal connector to a data acquisition board. See Chapter 2, *Configuration and Installation*, for more information. To make a measurement from another module, perform the following steps:

1. Perform any necessary programming to ensure that no modules are driving Analog Bus 0. For an SCXI-1121, clearing `AB0EN` in the Configuration Register will ensure that its output is not driving `AB0`.
2. Write the binary pattern `000XXXXX XX100011` to the SCXI-1121 Configuration Register. This step disables the SCXI-1121 from driving Analog Bus 0 and allows Analog Bus 0 to drive `MCH0` through the output buffer.
3. Program the other module to drive Analog Bus 0 with the signal to be measured.
4. Measure the voltage with the data acquisition board.

Measurements from the SCXI-1121 via Another Module

To perform measurements via another module, you must cable the other module rear signal connector to a data acquisition board. The other module must also be able to transfer Analog Bus 0 to the data acquisition board. See Chapter 2, *Configuration and Installation*, for more information.

To measure one of the four differential input channels to the SCXI-1121, perform the following steps:

1. Perform any necessary programming to ensure that no modules are driving Analog Bus 0. For an SCXI-1121, clearing ABOEN in the Configuration Register will ensure that its output is not driving AB0.
2. Program the other module not to drive Analog Bus 0, but to send Analog Bus 0 to the data acquisition board.
3. Write the binary pattern 000XXXCC XX000010 to the SCXI-1121 Configuration Register.
4. Measure the voltage with the data acquisition board.

To perform a shunt calibration on one of the four differential input channels of the SCXI-1121, perform the following steps:

1. Perform any necessary programming to ensure that no modules are driving Analog Bus 0. For an SCXI-1121, clearing ABOEN in the Configuration Register will ensure that its output is not driving AB0.
2. Program the other module not to drive Analog Bus 0, but to send Analog Bus 0 to the data acquisition board.
3. Write the binary pattern 001XXXCC XX000010 to the SCXI-1121 Configuration Register.
4. Insert a delay equal to 1 sec if you have set the 4 Hz filter, or 1 msec if you have set the 10 kHz filter. This delay permits the SCXI-1121 amplifier to settle.
5. Measure the voltage with the data acquisition board.

To measure the voltage on the MTEMP line, perform the following steps:

1. Perform any necessary programming to ensure that no modules are driving Analog Bus 0. For an SCXI-1121, clearing ABOEN in the Configuration Register will ensure that its output is not driving AB0.
2. Program the other module not to drive Analog Bus 0, but to send Analog Bus 0 to the data acquisition board.
3. Write the binary pattern 000XXXXX XX100010 to the SCXI-1121 Configuration Register.
4. Measure the voltage with the data acquisition board.

Scanning Measurements

Programming for scanned data acquisition involves programming your data acquisition board, modules, and Slot 0. In general, the steps to be taken are as follows:

1. Perform all data acquisition board programming to the point of enabling the data acquisition.
2. Perform all module programming.
3. Program the Slot 0 hardscan circuitry.
4. Enable the data acquisition, trigger it either through software or hardware, and service the data acquisition.

The MIO boards can do all types of scanning. Lab-NB, Lab-PC, Lab-PC+, Lab-LC, and PC-LPM-16 boards support only single-module parallel scanning, and do not support any of the multiplexed scanning modes. Notice that single-module parallel scanning is typically done without any module or Slot 0 programming; only programming the data acquisition board is necessary.

1. Data Acquisition Board Setup Programming

The programming steps for your data acquisition board are given in your data acquisition board user manual. You should follow the instructions in the following sections:

- *AT-MIO-16 User Manual*
 - *Multiple A/D Conversions with Continuous Channel Scanning (Round Robin)*
 - *Multiple A/D Conversions with Interval Channel Scanning (Pseudosimultaneous)*
- *AT-MIO-16D User Manual*
 - *Multiple A/D Conversions with Continuous Channel Scanning (Round Robin)*
 - *Multiple A/D Conversions with Interval Channel Scanning (Pseudosimultaneous)*
- *AT-MIO-16F-5 User Manual*
 - *Posttrigger Data Acquisition with Continuous Channel Scanning*
 - *Posttrigger Data Acquisition with Interval Channel Scanning*
- *AT-MIO-16X User Manual*
 - *Continuous Channel Scanning Data Acquisition*
 - *Interval Channel Scanning Data Acquisition*
- *AT-MIO-64F-5 User Manual*
 - *Continuous Channel Scanning Data Acquisition*
 - *Interval Channel Scanning Data Acquisition*

- *Lab-LC User Manual*
 - *Programming Multiple A/D Conversions with Channel Scanning*
- *Lab-NB User Manual*
 - *Programming Multiple A/D Conversions with Channel Scanning*
- *Lab-PC User Manual*
 - *Programming Multiple A/D Conversions with Channel Scanning*
- *Lab-PC+ User Manual*
 - *Programming Multiple A/D Conversions with Channel Scanning*
 - *Programming Multiple A/D Conversions with Interval Scanning*
 - *Programming Multiple A/D Conversions in Single-Channel Interval Acquisition Mode*
- *MC-MIO-16 User Manual*
 - *Multiple A/D Conversions with Continuous Channel Scanning (Round Robin)*
 - *Multiple A/D Conversions with Interval Channel Scanning (Pseudosimultaneous)*
- *NB-MIO-16 User Manual*
 - *Programming Multiple A/D Conversions with Channel Scanning*
- *NB-MIO-16X User Manual*
 - *Multiple A/D Conversions with Continuous Channel Scanning (Round Robin)*
 - *Multiple A/D Conversions with Interval Channel Scanning (Pseudosimultaneous)*
- *PC-LPM-16 User Manual*
 - *Programming Multiple A/D Conversions with Channel Scanning*

Follow the instructions in these sections through the part labeled as follows:

- *Clear the A/D Circuitry and Reset the Mux Counter* in the MIO board user manual (except for the AT-MIO-16X and the AT-MIO-64F-5). Do not continue to the part called *Enable the Scanning Data Acquisition Operation*. You will do this after you program the modules and Slot 0.
- *Program the Sample Counter* (if you are doing continuous channel scanning) or *Program the Scan-Interval Counter* (if you are doing interval channel scanning) in the AT-MIO-16X or AT-MIO-64F-5 user manual. Do not continue to the part labeled *Enable a Scanning Data Acquisition Operation* or *Enable an Interval Scanning Data Acquisition Operation*. You will do this after you program the modules and Slot 0.

Note: *For multiplexed scanning with an MIO board, it is important that you follow the instructions in the channel-scanning sections, not the single-channel sections. Although you may be using only one MIO board channel, the channel scanning programming will ensure that the MIO board outputs SCANCLK, which is needed by the SCXI-1120 and Slot 0.*

- *Clear the A/D Circuitry in the Lab-LC User Manual. Do not continue to the part called Program the Sample-Interval Counter. You will do this after you program the modules and Slot 0.*
- *Clear the A/D Circuitry in the Lab-PC User Manual, the Lab-PC+ User Manual, and the PC-LPM-16 User Manual. Do not continue to the part called Start and Service the Data Acquisition Operation. You will do this after you program the modules and Slot 0.*
- *Clear the A/D Circuitry in the Lab-NB User Manual. Do not continue to the part called Program the Sample-Interval Counter (Counter A0). You will do this after you program the modules and Slot 0.*

Counter 1 and SCANDIV

All MIO boards can operate their data acquisition board scan lists in two ways—they can acquire one sample per data acquisition board scan list entry; or they can acquire N samples per data acquisition board scan list entry, where N is a number from 2 to 65,535 that is programmed in Counter 1. This second method of operation is especially useful when the data acquisition board scan list length is limited to 16 entries, as it is on all MIO boards except the AT-MIO-16F-5, which can have up to 512 entries. Because you can multiplex many SCXI-1121s in one chassis to one MIO board channel, often the simplest way to program the MIO board is to use only one data acquisition board scan list entry, and make N the total number of samples to be taken on all modules in one scan. Check your MIO board user manual for limitations in the data acquisition board scan list format.

To program the MIO board to take N samples per data acquisition board scan list entry, perform the following additional programming steps at the end of the *Enable the Scanning Data Acquisition Operation* section in the appropriate data acquisition board user manual:

1. Write FF01 to the Am9513 Command Register to select Counter 1 Mode Register.
2. Write 0325 (hex) to the Am9513 Data Register to store Counter 1 Mode Value for most MIO boards. Write 1325 (hex) to the Am9513 Data Register to store Counter 1 Mode Value for the AT-MIO-16F-5, AT-MIO-64F-5, and AT-MIO-16X boards.
3. Write FF09 to the Am9513 Command Register to select Counter 1 Load Register.
4. Write the number of samples to be taken per scan list entry (2 to 65,535) to the Am9513 Data Register to load Counter 1.
5. Write FF41 to the Am9513 Command Register to load Counter 1.
6. Write FFF1 to the Am9513 Command Register to step Counter 1.
7. Write FF21 to the Am9513 Command Register to arm Counter 1.
8. Set the SCANDIV bit in Command Register 1.

2. Module Programming

This section describes the programming steps for various scanning possibilities. For all the bit patterns in this section, S_C signifies the shunt calibration bit. If you set this bit to one, the module will be scanned in Shunt Calibration mode. If you clear this bit to zero, shunt calibration will be disabled on the module during scanning. When programming a module to change the shunt calibration mode from disabled to enabled or vice versa, insert a delay before you make any measurements. If the SCXI-1121 has a filter setting at 10 kHz, the delay should be at least 1 msec. If the SCXI-1121 has the filter set at 4 Hz, the delay should be at least 1 sec.

Single-Module Parallel Scanning

In order to perform single-module parallel scanning, you must cable the SCXI-1121 rear signal connector to a data acquisition board with each output connected to a different data acquisition board channel. See Chapter 2, *Configuration and Installation*, for more information.

To program the SCXI-1121 for single-module parallel scanning, write the binary pattern $00S_CXXX00\ XX000000$ to the SCXI-1121 Configuration Register. Notice that this can be the RESET state.

Single-Module Multiplexed Scanning (Direct)

To perform simple channel scanning, you must cable the SCXI-1121 to a data acquisition board. See Chapter 2, *Configuration and Installation*, for more information.

To program the module for scanned channel measurements, write the binary pattern $10S_CXXXCC\ XX001101$ to the SCXI-1121 Configuration Register. CC represents the starting channel number.

Single-Module Multiplexed Scanning (Indirect)

To indirectly scan a module, send the output of the scanned module onto Analog Bus 0, where it will be picked up by another module and transmitted to the data acquisition board.

Channel Scanning from Other Modules. To scan measurements from other modules, you must cable the SCXI-1121 to a data acquisition board. See Chapter 2, *Configuration and Installation*, for more information. The module programming steps are as follows:

1. Perform any necessary programming to ensure that no modules are driving Analog Bus 0. For an SCXI-1121, clearing ABOEN in the Configuration Register will ensure that its output is not driving AB0.
2. Write the binary pattern $10XXXXXX\ XX100011$ to the SCXI-1121 Configuration Register. This step disables the SCXI-1121 from driving Analog Bus 0 and allows Analog Bus 0 to drive MCH0 through the output buffer.
3. Program the other module to be scanned.

Channel Scanning from the SCXI-1121 via Another Module. To scan the SCXI-1121 via other modules, you must cable the other module to a data acquisition board and the other module must be able to transfer Analog Bus 0 to the data acquisition board. The other module must also be able to send a SCANCLK*-compatible signal on TRIG0. See Chapter 2, *Configuration and Installation*, for more information. The module programming steps are as follows:

1. Perform any necessary programming to ensure that no modules are driving Analog Bus 0. For an SCXI-1121, clearing ABOEN in the Configuration Register will ensure that its output is not driving AB0.
2. Program the other module not to drive Analog Bus 0, but to send Analog Bus 0 to the data acquisition board. Also program the other module to send a SCANCLK*-compatible signal to TRIG0.
3. Write the binary pattern $01S_CXXXCC \ XX001111$ to the SCXI-1121 Configuration Register, where CC is the starting channel number.

Multiple-Module Multiplexed Scanning

To scan multiple modules, you must connect one module to the data acquisition board and the module must be able to transfer Analog Bus 0 to the data acquisition board. This module must also be able to send a SCANCLK*-compatible signal on TRIG0. See Chapter 2, *Configuration and Installation*, for more information. The module programming steps are as follows:

1. Perform any necessary programming to ensure that no modules are driving Analog Bus 0. For an SCXI-1121, clearing ABOEN in the Configuration Register will ensure that its output is not driving AB0.
2. Program the module that is connected to the data acquisition board to connect Analog Bus 0 to the data acquisition board but not drive Analog Bus 0 unless it is receiving an active low signal on SCANCON. Also program the module to send a SCANCLK*-compatible signal onto TRIG0. If this module is an SCXI-1121, this programming is accomplished by writing the binary pattern $10S_CXXXCC \ XX001111$ to its Configuration Register.

Note: *If this module is an SCXI-1121 and is not going to be scanned (it is just being used as an interface), write a zero to bit 2 (SCANCONEN) in the Configuration Register. The start channel bits become don't care bits.*

3. Program the other modules to be used in the scan to connect their outputs to Analog Bus 0 but not to drive Analog Bus 0 unless receiving an active low signal on SCANCON. Also program the other modules to use TRIG0 as their clock source. For SCXI-1121 modules, this programming is accomplished by writing the binary pattern $01S_CXXXCC \ XX001111$ to their Configuration Registers.

Multiple-Chassis Scanning

To scan modules on multiple chassis, you must use the SCXI-1001. The cable from the data acquisition board must bus the digital lines to one module on each chassis. Additionally, the cable must provide each chassis with its own analog channel. The data acquisition board must be able to take several readings at a time on a given channel before accessing a new channel. See the *Counter 1 and SCANDIV* subsection of the *Data Acquisition Board Setup Programming* section earlier in this chapter. You can use the MIO-16 boards in conjunction with the SCXI-1350 multichassis adapter for multichassis scanning.

For each chassis, program the modules according to the appropriate mode of operation, disregarding the fact that other chassis will be involved.

For example, you want to scan thirteen modules. Twelve modules are in one chassis. The thirteenth is in the second chassis and is to be scanned through a fourteenth module that is cabled to the data acquisition board but is not involved in the scan. Program the twelve modules in the first chassis according to the steps in the previous *Multiple-Module Multiplexed Scanning* section, and program the thirteenth and fourteenth modules according to *Channel Scanning from the SCXI-1121 via Another Module* earlier in this chapter.

3. Programming the Slot 0 Hardscan Circuitry

The following section describes how to program the Slot 0 circuitry for scanning operations. For a more detailed description of the Slot 0 scanning circuitry, consult the *SCXI-1000/1001 User Manual*. Descriptions of the Slot 0 registers are given in the section *Slot 0 Register Descriptions* in Chapter 4, *Register Descriptions*. Skip this section if you are doing single-module parallel scanning.

To program the hardscan circuitry, perform the following steps:

1. Write binary 0000 0000 to the HSCR.
2. Write binary 0000 1000 to the HSCR.
3. Write the Slot 0 scan list to the FIFO.
4. Write binary 0010 1100 to the HSCR.
5. Write binary 101S 1100 to the HSCR.
6. Write binary 101S 1110 to the HSCR.
7. Write binary 101S 1111 to the HSCR.

To program the hardscan circuitry to use the current scan list, perform the following steps:

1. Write binary 0000 1000 to the HSCR.
2. Write binary 0100 1000 to the HSCR.
3. Write binary 0000 1000 to the HSCR.
4. Write binary 0010 1100 to the HSCR.
5. Write binary 101S 1100 to the HSCR.

6. Write binary 101S 1110 to the HSCR.
7. Write binary 101S 1111 to the HSCR.

In the preceding steps, $S = 0$ if you want the scanning to repeat when the end of the list is reached. $S = 1$ if you want the circuitry to shut down after a single scan.

When you are writing multiple entries to the same register, for example, repetitive writes to the HSCR or several FIFO entries, it is important that SS*13 or SS*14 go inactive (high) between each entry. Select another slot or toggle the SLOTOSEL* line to temporarily deassert the appropriate SS* line.

If consecutive scan list entries access an SCXI-1121, the module will reload the MUXCOUNTER with the starting channel after each entry. Thus, two entries with counts of two for one module will yield different behavior than one entry with a count of four.

For multiple-chassis scanning, program each Slot 0 with dummy entries to fill the sample counts when the data acquisition board is accessing other chassis. Use Slot 13 as the dummy entry slot. See *Example 3* at the end of this chapter.

4. Acquisition Enable, Triggering, and Servicing

At this point, you should now continue from where you left off in the *Data Acquisition Board Setup Programming* section of this chapter. Perform the following steps given in your data acquisition board user manual.

- MIO board user manual
 - Enable the scanning data acquisition operation.
 - Apply a trigger.
 - Service the data acquisition operation.
- *Lab-PC User Manual, Lab-PC+ User Manual, and PC-LPM-16 User Manual*
 - Start and service the data acquisition operation.
- *Lab-LC User Manual*
 - Program the sample-interval counter.
 - Service the data acquisition operation.
- *Lab-NB User Manual*
 - Program the sample-interval counter (Counter A0)
 - Service the data acquisition operation.

Scanning Examples

The following examples are intended to aid your understanding of module and Slot 0 programming. It will be helpful to refer to the bit descriptions for the Configuration Register and the FIFO Register at the beginning of Chapter 4, *Register Descriptions*.

Example 1

You want to scan, in Multiplexed mode, channels 1 through 3 on an SCXI-1121 in Slot 1 of an SCXI-1000 chassis. The SCXI-1121 is directly cabled to a data acquisition board.

The programming steps are as follows:

1. Program your data acquisition board as described in the *Data Acquisition Board Setup Programming* section of this chapter.
2. Following the procedure given in the *Register Writes* section, write 10000001 00001101 to the Configuration Register of the SCXI-1121 in Slot 1.
3. Follow the steps outlined in the section earlier in this chapter, *3. Programming the Slot 0 Hardscan Circuitry*, where step 3, *Write the Slot 0 scan list to the FIFO*, consists of the following:

Write 00000000 00000010 to the FIFO Register. This corresponds to Slot 1 for three samples.

4. Follow the procedure given in the section, *4. Acquisition Enable, Triggering, and Servicing*, earlier in this chapter.

Example 2

An SCXI-1000 chassis has four SCXI-1121s in Slots 1, 2, 3, and 4. The SCXI-1121 in Slot 4 is cabled to the data acquisition board. You want to scan channels 1 through 3 on the SCXI-1121 in Slot 1, channels 0 and 1 on the SCXI-1121 in Slot 4, and channels 3 and 2 on the SCXI-1121 in Slot 3.

The programming steps are as follows:

1. Program your data acquisition board as described in the *Data Acquisition Board Setup Programming* section.
2. Following the procedure given in the *Register Writes* section, write 00000000 00000000 to the Configuration Register of the SCXI-1121 in Slot 2. This step resets the module, including the clearing of the AB0EN bit (bit 0). Notice that a complete reset of this module is not necessary, but is used for simplicity.
3. Following the procedure given in the *Register Writes* section, write 100XXX00 00001111 to the Configuration Register of the SCXI-1121 in Slot 4.

4. Following the procedure given in the *Register Writes* section, write 010XXX01 00001111 to the Configuration Register of the SCXI-1121 in Slot 1.
5. Following the procedure given in the *Register Writes* section, write 010XXX11 00001111 to the Configuration Register of the SCXI-1121 in Slot 3. Notice that after Channel 3, the SCXI-1121 will *wrap around* to Channel 0.
6. Follow the steps given in the section earlier in this chapter, *3. Programming the Slot 0 Hardscan Circuitry*, where step 3, *Write the Slot 0 scan list to the FIFO*, consists of the following:
 - a. Write 00000000 00000010 to the FIFO Register. This corresponds to Slot 1 for three samples.
 - b. Write 00000001 10000001 to the FIFO Register. This corresponds to Slot 4 for two samples.
 - c. Write 00000001 00000011 to the FIFO Register. This corresponds to Slot 3 for four samples.

Make sure to toggle SLOT0SEL* or reselect the FIFO Register from scratch between steps 6a, 6b, and 6c.
7. Follow the procedure given in the *4. Acquisition Enable, Triggering, and Servicing* section earlier in this chapter.

Example 3

You want to scan four channels on an SCXI-1121 in Slot 4 of Chassis 1, then two channels of an SCXI-1121 in Slot 11 of Chassis 2, one channel of an SCXI-1121 in Slot 3 in Chassis 3, and three channels of an SCXI-1121 in Slot 8 of Chassis 3.

Assuming that the modules are cabled and programmed correctly, the Slot 0 scan lists should be as follows:

Chassis 1			Chassis 2			Chassis 3		
Entry	Slot Number	Count	Entry	Slot Number	Count	Entry	Slot Number	Count
1	4	4	1	13	4	1	13	6
2	13	6	2	11	2	2	3	1
			3	13	4	3	8	3

Other solutions are possible.

In the section, *3. Programming the Slot 0 Hardscan Circuitry*, earlier in this chapter, step 3 consists of the following steps:

1. Select Slot 14 in Chassis 1.
2. Write `XXXXX001 10000011` over MOSI.
3. Toggle SLOTOSEL*.
4. Write `XXXXX110 00000101` over MOSI.
5. Select Slot 14 in Chassis 2.
6. Write `XXXXX110 00000011` over MOSI.
7. Toggle SLOTOSEL*.
8. Write `XXXXX101 00000001` over MOSI.
9. Toggle SLOTOSEL*.
10. Write `XXXXX110 00000011` over MOSI.
11. Select Slot 14 in Chassis 3.
12. Write `XXXXX110 00000101` over MOSI.
13. Toggle SLOTOSEL*.
14. Write `XXXXX001 00000000` over MOSI.
15. Toggle SLOTOSEL*.
16. Write `XXXXX011 10000010` over MOSI.
17. Select Slot 0 in Chassis 0.

Appendix A

Specifications

This appendix lists the specifications for the SCXI-1121. These are typical at 25° C unless otherwise stated. The operating temperature range is 0° to 50° C.

Analog Input

Gain (jumper-selectable)	1, 2, 5, 10, 20, 50, 100, 200, 500, 1,000, 2,000
Output range	±5 V
Number of channels	4
Gain accuracy ¹	0.15% of full scale
Offset voltage	
Input	±6 µV
Output	±3 mV
Stability versus ambient temperature	
Input offset drift	±0.2 µV/°C
Output offset drift	±200 µV/°C
Gain drift	20 ppm/°C
Input bias current	±80 pA
Input resistance	
Normal	40 MΩ
Power off	50 kΩ
Overload	50 kΩ
Output resistance	
Multiplexed-Output mode	100 Ω
Parallel-Output mode	330 Ω
Filtering (jumper-selectable)	4 Hz (-10 dB) or 10 kHz (-3 dB), 3-pole RC
Noise (400 kHz bandwidth) ²	
Input (gain = 1,000)	
4 Hz filter	100 nVrms
10 kHz filter	4 µVrms
Output (gain = 1)	
4 Hz	150 µVrms
10 kHz	1 mVrms

¹ Includes the combined effects of gain, offset, and hysteresis and nonlinearity

² Includes the combined effects of the SCXI-1121 and the AT-MIO-16F-5

Output selection time (with 5 V step, all gains) ²	
0.012% accuracy	5.2 μ sec typical, 7 μ sec maximum
0.006% accuracy	10 μ sec
0.0015% accuracy	20 μ sec
Rise time	
4 Hz	0.12 sec
10 kHz	70 μ sec
Slew rate	0.15 V/ μ sec
Operating common-mode voltage, 50 Hz or 60 Hz	
Channel to channel or Channel to earth	250 Vrms ³
Common-mode rejection ratio, 50 or 60 Hz	
1 k Ω in input leads	160 dB minimum at 4 Hz bandwidth
NMR (50 or 60 Hz)	60 dB at 4 Hz bandwidth
Input protection (continuous)	250 Vrms maximum
Output protection	Continuous short-to-ground
Power dissipation	7.5 W maximum

RTD Mode

Excitation current	0.15 mA \pm 0.04%, 0.45 mA \pm 0.2%
Maximum load resistance	10 k Ω
Drift	40 ppm/ $^{\circ}$ C
Lead resistance effect	Negligible (4-wire measurement)
Resistance range	10 k Ω , maximum

Strain Gauge Mode

Bridge types	Quarter-, half-, and full-bridge
Bridge completion	Two 4.5 k Ω \pm 0.05% ratio tolerance resistors

¹Includes the combined effects of gain, offset, and hysteresis and nonlinearity

²Includes the combined effects of the SCXI-1121 and the AT-MIO-16F-5

³Module tested following the UL 1244 standard to twice the working voltage +1000 Vrms

Excitation voltage	3.333 V \pm 0.04% or 10 V \pm 0.2%
Resistance range	120 Ω , minimum at 3.333 V; 800 Ω , minimum at 10 V
Half-bridge voltage	$V_{EXT}/2 \pm 0.04\%$

Cold-Junction Sensor⁴

SCXI-1320 and SCXI-1321

Accuracy	1.0° C over 0° to 55° C
Output	10 mV/°C

SCXI-1328

Accuracy ⁵	0.35° from 15° to 35° C 0.65° from 0° to 15° and 35° to 55° C
Output	1.91 to 0.58 V from 0° to 55° C
Output at 25° C	1.25 V

Note: You can find the temperature T (°C) as follows:

$$T = T_K - 273.15$$

where T_K is the temperature in kelvin

$$T_K = \frac{1}{\left[a + b(\ln R_T) + c(\ln R_T)^3 \right]}$$

$$a = 1.288 \times 10^{-3}$$

$$b = 2.356 \times 10^{-4}$$

$$c = 9.556 \times 10^{-8}$$

R_T = resistance of the thermistor in Ω

$$R_T = 50,000 \left(\frac{V_{TEMPOUT}}{2.5 - V_{TEMPOUT}} \right)$$

$V_{TEMPOUT}$ = output voltage of the temperature sensor

Physical

Dimensions	1.2 by 6.8 by 8.0 in.
Connectors	50-pin male ribbon-cable rear connector 32-pin DIN C front connector (18-screw terminal adapter available)

⁴Located on the SCXI-1320, SCXI-1328, and SCXI-1321 terminal blocks

⁵Includes the combined effects of the temperature sensor accuracy and the temperature difference between the temperature sensor and any screw terminal

Operating Environment

Temperature	0 to 50° C
Relative humidity	5% to 90% at 35° C

Storage Environment

Temperature	-55° to 150° C -55° to 125° C for SCXI-1328
Relative humidity	5% to 90% noncondensing

Appendix B

Rear Signal Connector

This appendix describes the pinout and signal names for the SCXI-1121 50-pin rear signal connector, including a description of each connection.

Figure B-1 shows the pin assignments for the SCXI-1121 rear signal connector.

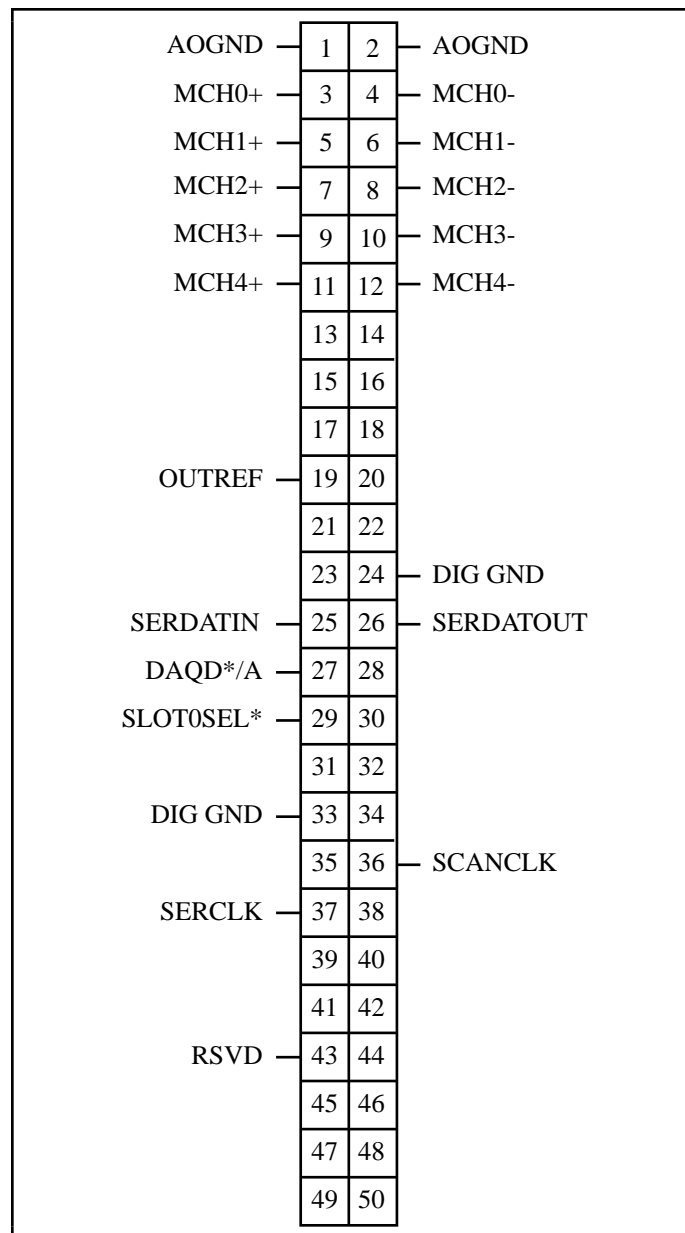


Figure B-1. SCXI-1121 Rear Signal Connector Pin Assignment

Rear Signal Connector Signal Descriptions

Pin	Signal Name	Description
1-2	AOGND	Analog Output Ground – These pins are connected to the analog reference when jumper W33 is in position AB-R0.
3-12	MCH0± through MCH4±	Analog Output Channels 0 through 4 – Connects to the data acquisition board differential analog input channels.
19	OUTREF	Output Reference – This pin serves as the reference node for the analog channels output in the Pseudodifferential Reference mode. It should be connected to the analog input sense of the NRSE data acquisition board.
24, 33	DIG GND	Digital Ground – These pins supply the reference for data acquisition board digital signals and are tied to the module digital ground.
25	SERDATIN	Serial Data In – This signal taps into the SCXIBus MOSI line to provide serial input data to a module or Slot 0.
26	SERDATOUT	Serial Data Out – This signal taps into the SCXIBus MISO line to accept serial output data from a module.
27	DAQD*/A	Data Acquisition Board Data/Address Line – This signal taps into the SCXIBus D*/A line to indicate to the module whether the incoming serial stream is data or address information.
29	SLOT0SEL*	Slot 0 Select – This signal taps into the SCXIBus INTR* line to indicate whether the information on MOSI is being sent to a module or Slot 0.
36	SCANCLK	Scan Clock – This indicates to the SCXI-1121 that a sample has been taken by the data acquisition board and causes the SCXI-1121 to change channels.
37	SERCLK	Serial Clock – This signal taps into the SCXIBus SPICLK line to clock the data on the MOSI and MISO lines. See the <i>Timing Requirements and Communication Protocol</i> section later in this chapter for more detailed information on timing.
43	RSVD	Reserved.

All other pins are not connected.

See the *Timing Requirements and Communication Protocol* section in Chapter 2, *Configuration and Installation*, for more detailed information on timing. Detailed signal specifications are also included in Chapter 2.

Appendix C

SCXIBus Connector

This appendix describes the pinout and signal names for the SCXI-1121 96-pin SCXIBus connector, including a description of each connection.

Figure C-1 shows the pin assignments for the SCXI-1121 SCXIBus connector.

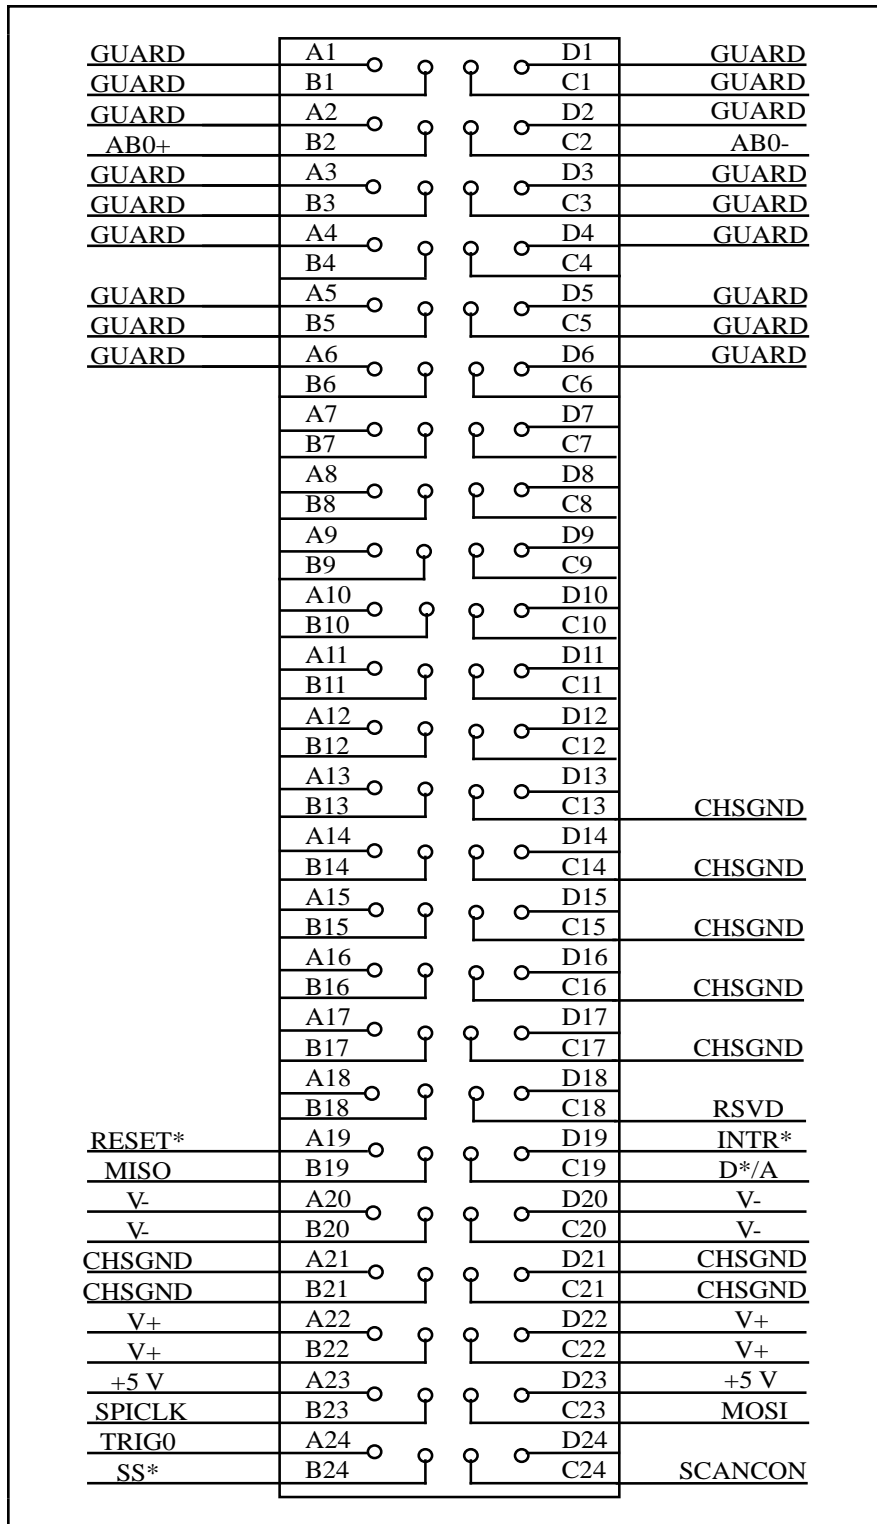


Figure C-1. SCXibus Connector Pin Assignment

SCXIBus Connector Signal Descriptions

Pin	Signal Name	Description
A1, B1, C1, D1, A2, D2, A3, B3, C3, D3, A4, D4, A5, B5, C5, D5, A6, D6	GUARD	Guard – Shields and guards the analog bus lines from noise.
B2	AB0+	Analog Bus 0+ – Positive analog bus 0 line. Used to multiplex several modules to one analog signal.
C2	AB0-	Analog Bus 0- – Negative analog bus 0 line. Used to multiplex several modules to one analog signal.
C13-C17, A21, B21, C21, D21	CHSGND	Chassis Ground – Digital and analog ground reference.
C18	RSVD	Reserved.
A19	RESET*	Reset – When pulled low, reinitializes the module to its power-up state. Totem pole. Input.
B19	MISO	Master-In Slave-Out – Transmits data from the module to the SCXIBus. Open collector. I/O.
C19	D*/A	Data/Address – Indicates to the module whether address information or data information is being sent to the module on MOSI. Open collector. I/O.
D19	INTR*	Interrupt – Active low. Causes data that is on MOSI to be written to the Slot-Select Register in Slot 0. Open collector. Output.
A20, B20, C20, D20	V-	Negative Analog Supply – -18.5 to -25 V.
A22, B22, C22, D22	V+	Positive Analog Supply – +18.5 to +25 V.
A23, D23	+5 V	+5 VDC Source – Digital power supply.
B23	SPICLK	Serial Peripheral Interface (SPI) Clock – Clocks the serial data on the MOSI and MISO lines. Open collector. I/O.
C23	MOSI	Master-Out Slave-In – Transmits data from the SCXIBus to the module. Open collector. I/O.

Pin	Signal Name	Description (continued)
A24	TRIG0	TRIG0 – General-purpose trigger line used by the SCXI-1121 to send SCANCLK to other modules or receive SCANCLK from other modules. Open collector. I/O.
B24	SS*	Slot Select – When low, enables module communications over the SCXIBus. Totem pole. Input.
C24	SCANCON	Scanning Control – Combination output enable and reload signal for scanning operations. Totem pole. Input.

All other pins are not connected.

Further information is given in Chapter 3, *Theory of Operation*.

Appendix D

SCXI-1121 Front Connector

This appendix describes the pinout and signal names for the SCXI-1121 front connector, including a description of each connection.

Figure D-1 shows the pin assignments for the SCXI-1121 front connector.

Pin Number	Signal Name	Column			Signal Name
		A	B	C	
32	CH0+	○	○	○	CH0-
31		○	○	○	
30	EX0+	○	○	○	EX0+
29		○	○	○	
28	EGND0	○	○	○	
27		○	○	○	
26	CH1+	○	○	○	CH1-
25		○	○	○	
24	EX1+	○	○	○	EX1-
23		○	○	○	
22	EGND1	○	○	○	
21		○	○	○	
20	CH2+	○	○	○	CH2-
19		○	○	○	
18	EX2+	○	○	○	EX2-
17		○	○	○	
16	EGND2	○	○	○	
15		○	○	○	
14	CH3+	○	○	○	CH3-
13		○	○	○	
12	EX3+	○	○	○	EX3-
11		○	○	○	
10	EGND3	○	○	○	
9		○	○	○	
8		○	○	○	RSVD
7		○	○	○	
6	SCAL	○	○	○	RSVD
5		○	○	○	
4	+5 V	○	○	○	MTEMP
3		○	○	○	
2	CGND	○	○	○	DTEMP
1		○	○	○	

Figure D-1. SCXI-1121 Front Connector Pin Assignment

Front Connector Signal Descriptions

Pin	Signal Name	Description
A2	CGND	Chassis Ground – This pin is tied to the SCXI chassis.
C2	DTEMP	Direct Temperature Sensor – This pin connects the temperature sensor to the MCH4+ when the terminal block is configured for direct temperature connection.
A4	+5 V	+5 VDC Source – This pin is used to power the temperature sensor on the terminal block. 0.2 mA of source not protected.
C4	MTEMP	Multiplexed Temperature Sensor – This pin connects the temperature sensor to the output multiplexer.
A6	SCAL	Shunt Calibration – This pin is tied to the SCAL bit and is used to control the SCXI-1321 shunt calibration switch. CMOS/TTL output; not protected.
C6, C8	RSVD	Reserved – These pins are reserved. Do not connect any signal to these pins.
A8, C10, C16, C22, C28	No Connect	<i>Do not</i> connect any signal to these pins.
A10	EGND3	Excitation Ground 3 – This pin connects to the excitation ground 3 via a 51 k Ω resistor.
A12	EX3+	Positive Excitation Output 3 – This pin is connected to the excitation channel 3 positive output.
C12	EX3-	Negative Excitation Output 3 – This pin is connected to the excitation channel 3 negative output.
A14	CH3+	Positive Input Channel 3 – This pin is connected to the input channel 3 positive input.
C14	CH3-	Negative Input Channel 3 – This pin is connected to the input channel 3 negative input.
A16	EGND2	Excitation Ground 2 – This pin connects to the excitation ground 2 via a 51 k Ω resistor.

Pin	Signal Name	Description (continued)
A18	EX2+	Positive Excitation Output 2 – This pin is connected to the excitation channel 2 positive output.
C18	EX2-	Negative Excitation Output 2 – This pin is connected to the excitation channel 2 negative output.
A20	CH2+	Positive Input Channel 2 – This pin is connected to the input channel 2 positive input.
C20	CH2-	Negative Input Channel 2 – This pin is connected to the input channel 2 negative input.
A22	EGND1	Excitation Ground 1 – This pin connects to the excitation ground 1 via a 51 k Ω resistor.
A24	EX1+	Positive Excitation Output 1 – This pin is connected to the excitation channel 1 positive output.
C24	EX1-	Negative Excitation Output 1 – This pin is connected to the excitation channel 1 negative output.
A26	CH1+	Positive Input Channel 1 – This pin is connected to the input channel 1 positive input.
C26	CH1-	Negative Input Channel 1 – This pin is connected to the input channel 1 negative input.
A28	EGND0	Excitation Ground 0 – This pin connects to the excitation ground 0 via a 51 k Ω resistor.
A30	EX0+	Positive Excitation Output 0 – This pin is connected to the excitation channel 0 positive output.
C30	EX0-	Negative Excitation Output 0 – This pin is connected to the excitation channel 0 negative output.
A32	CH0+	Positive Input Channel 0 – This pin is connected to the input channel 0 positive input.
C32	CH0-	Negative Input Channel 0 – This pin is connected to the input channel 0 negative input.

Further information is given in Chapter 2, *Configuration and Installation*.

Appendix D

SCXI-1121 Front Connector

This appendix describes the pinout and signal names for the SCXI-1121 front connector, including a description of each connection.

Figure D-1 shows the pin assignments for the SCXI-1121 front connector.

Pin Number	Signal Name	Column			Signal Name
		A	B	C	
32	CH0+	○	○	○	CH0-
31		○	○	○	
30	EX0+	○	○	○	EX0+
29		○	○	○	
28	EGND0	○	○	○	
27		○	○	○	
26	CH1+	○	○	○	CH1-
25		○	○	○	
24	EX1+	○	○	○	EX1-
23		○	○	○	
22	EGND1	○	○	○	
21		○	○	○	
20	CH2+	○	○	○	CH2-
19		○	○	○	
18	EX2+	○	○	○	EX2-
17		○	○	○	
16	EGND2	○	○	○	
15		○	○	○	
14	CH3+	○	○	○	CH3-
13		○	○	○	
12	EX3+	○	○	○	EX3-
11		○	○	○	
10	EGND3	○	○	○	
9		○	○	○	
8		○	○	○	RSVD
7		○	○	○	
6	SCAL	○	○	○	RSVD
5		○	○	○	
4	+5 V	○	○	○	MTEMP
3		○	○	○	
2	CGND	○	○	○	DTEMP
1		○	○	○	

Figure D-1. SCXI-1121 Front Connector Pin Assignment

Front Connector Signal Descriptions

Pin	Signal Name	Description
A2	CGND	Chassis Ground – This pin is tied to the SCXI chassis.
C2	DTEMP	Direct Temperature Sensor – This pin connects the temperature sensor to the MCH4+ when the terminal block is configured for direct temperature connection.
A4	+5 V	+5 VDC Source – This pin is used to power the temperature sensor on the terminal block. 0.2 mA of source not protected.
C4	MTEMP	Multiplexed Temperature Sensor – This pin connects the temperature sensor to the output multiplexer.
A6	SCAL	Shunt Calibration – This pin is tied to the SCAL bit and is used to control the SCXI-1321 shunt calibration switch. CMOS/TTL output; not protected.
C6, C8	RSVD	Reserved – These pins are reserved. Do not connect any signal to these pins.
A8, C10, C16, C22, C28	No Connect	<i>Do not</i> connect any signal to these pins.
A10	EGND3	Excitation Ground 3 – This pin connects to the excitation ground 3 via a 51 k Ω resistor.
A12	EX3+	Positive Excitation Output 3 – This pin is connected to the excitation channel 3 positive output.
C12	EX3-	Negative Excitation Output 3 – This pin is connected to the excitation channel 3 negative output.
A14	CH3+	Positive Input Channel 3 – This pin is connected to the input channel 3 positive input.
C14	CH3-	Negative Input Channel 3 – This pin is connected to the input channel 3 negative input.
A16	EGND2	Excitation Ground 2 – This pin connects to the excitation ground 2 via a 51 k Ω resistor.

Pin	Signal Name	Description (continued)
A18	EX2+	Positive Excitation Output 2 – This pin is connected to the excitation channel 2 positive output.
C18	EX2-	Negative Excitation Output 2 – This pin is connected to the excitation channel 2 negative output.
A20	CH2+	Positive Input Channel 2 – This pin is connected to the input channel 2 positive input.
C20	CH2-	Negative Input Channel 2 – This pin is connected to the input channel 2 negative input.
A22	EGND1	Excitation Ground 1 – This pin connects to the excitation ground 1 via a 51 k Ω resistor.
A24	EX1+	Positive Excitation Output 1 – This pin is connected to the excitation channel 1 positive output.
C24	EX1-	Negative Excitation Output 1 – This pin is connected to the excitation channel 1 negative output.
A26	CH1+	Positive Input Channel 1 – This pin is connected to the input channel 1 positive input.
C26	CH1-	Negative Input Channel 1 – This pin is connected to the input channel 1 negative input.
A28	EGND0	Excitation Ground 0 – This pin connects to the excitation ground 0 via a 51 k Ω resistor.
A30	EX0+	Positive Excitation Output 0 – This pin is connected to the excitation channel 0 positive output.
C30	EX0-	Negative Excitation Output 0 – This pin is connected to the excitation channel 0 negative output.
A32	CH0+	Positive Input Channel 0 – This pin is connected to the input channel 0 positive input.
C32	CH0-	Negative Input Channel 0 – This pin is connected to the input channel 0 negative input.

Further information is given in Chapter 2, *Configuration and Installation*.

Appendix E

SCXI-1121 Cabling

This appendix describes how to use and install the hardware accessories for the SCXI-1121:

- SCXI-1340 cable assembly
- SCXI-1341 Lab-NB, Lab-PC, and Lab-PC+ cable assembly
- SCXI-1344 Lab-LC cable assembly
- SCXI-1342 PC-LPM-16 cable assembly
- SCXI-1180 feedthrough panel
- SCXI-1302 50-pin terminal block
- SCXI-1351 one-slot cable extender
- SCXI-1350 multichassis adapter
- SCXI-1343 screw terminal adapter

SCXI-1340 Cable Assembly

The SCXI-1340 cable assembly connects an MIO-16 board to an SCXI-1121 module. The SCXI-1340 consists of a 50-conductor ribbon cable that has mounting bracket at one end and a 50-pin female connector at the other end. The female connector connects to the I/O connector of the MIO-16 board. Attached to the mounting bracket is a 50-pin female mounting-bracket connector that connects to the module rear signal connector. To extend the signals of the MIO-16 board to an SCXI-1180 feedthrough panel or an SCXI-1181 breadboard module, you can use the male breakout connector that is near the mounting bracket on the ribbon cable. All 50 pins from the MIO-16 board go straight through to the rear signal connector. You can use a standard 50-pin ribbon cable instead of the SCXI-1340 cable assembly. The SCXI-1340 has the following advantages over the ribbon cable:

- The SCXI-1340 has strain relief so that you cannot accidentally disconnect the cable.
- The SCXI-1340 includes a mounting bracket that mounts to the chassis so that you can remove and reinsert the module without explicitly removing the cable from the back of the chassis. This is especially useful when the SCXI chassis is rack mounted, making rear access difficult.
- The SCXI-1340 has an extra male breakout connector for use with the SCXI-1180 feedthrough panel or additional modules or breadboards that need a direct connection to the MIO-16 board.
- The SCXI-1340 rear panel gives the module and the chassis both mechanical and electrical shielding.

Table E-1 lists the pin equivalences of the MIO-16 and the SCXI-1121.

Table E-1. SCXI-1121 and MIO-16 Pinout Equivalences

Pin	SCXI-1121 Rear Signal Connector	MIO-16 Equivalent
1-2	AOGND	AIGND
3	MCH 0+	ACH0
4	MCH 0-	ACH8
5	MCH 1+	ACH1
6	MCH 1-	ACH9
7	MCH2+	ACH2
8	MCH2-	ACH10
9	MCH3+	ACH3
10	MCH3-	ACH11
11	MCH4+	ACH4
12	MCH4-	ACH12
19	OUTREF	AISENSE
24, 33	DIG GND	DIG GND
25	SERDATIN	ADIO0
26	SERDATOUT	BDIO0
27	DAQD*/A	ADIO1
29	SLOT0SEL*	ADIO2
36	SCANCLK	SCANCLK
37	SERCLK	EXTSTROBE*
43	RSVD	OUT1

No other pins are connected on the SCXI-1121.

SCXI-1340 Installation

Follow these steps to install the SCXI-1340.

1. Make sure that the computer and the SCXI chassis are turned off.
2. Install the SCXI module in the chassis.
3. Plug the mounting bracket connector onto the module rear signal connector (see Figure E-1). Make sure the alignment tab on the bracket enters the upper board guide of the chassis.
4. Screw the mounting bracket to the threaded strips in the rear of the chassis.
5. Connect the loose end of the cable assembly to the MIO-16 board rear signal connector.

Check the installation.

After step 1, the order of these steps is not critical; however, it is easier to locate the correct position for the mounting bracket with a module installed in the chassis. If you will attach a cable to the breakout connector, installation is easiest if you attach the second cable before installing the SCXI-1340.

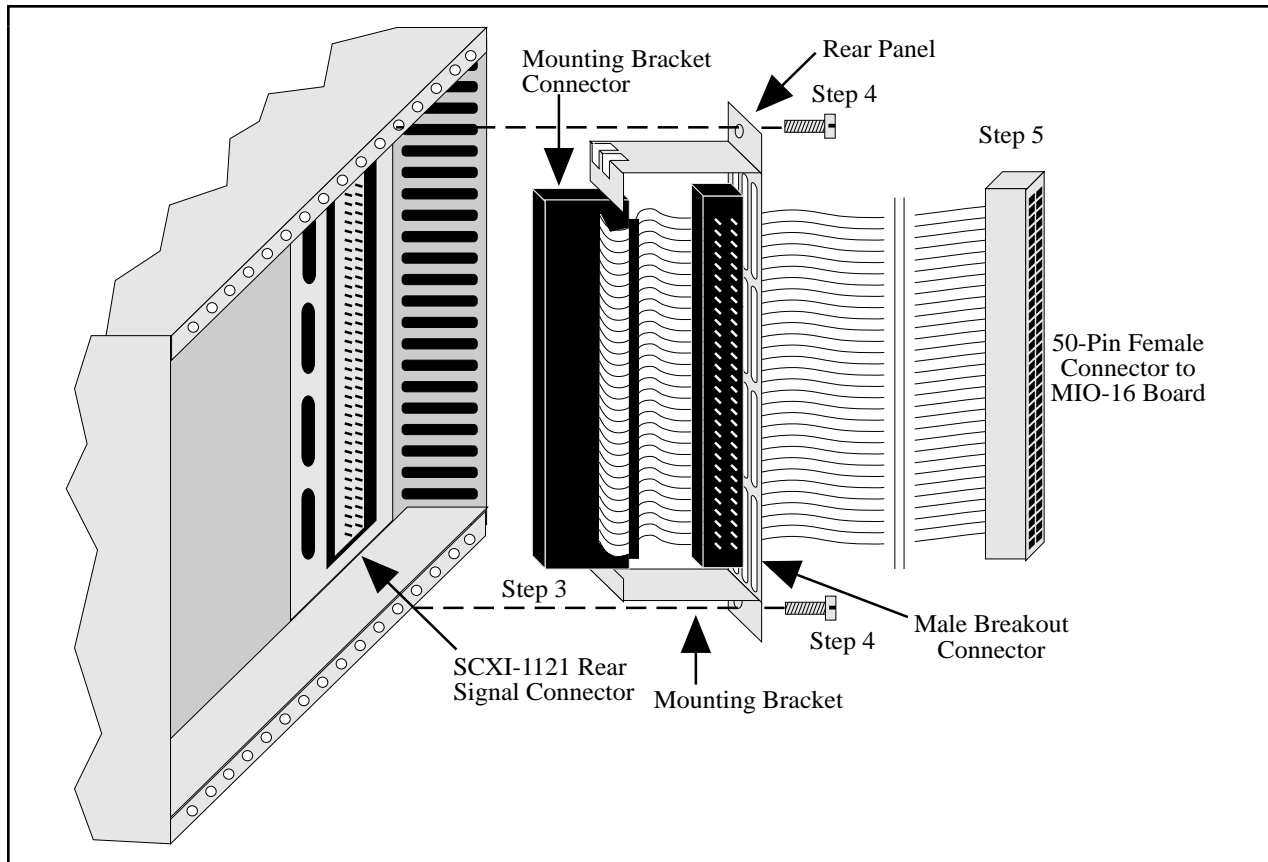


Figure E-1. SCXI-1340 Installation

SCXI-1341 Lab-NB, Lab-PC, or Lab-PC+ and SCXI-1344 Lab-LC Cable Assembly

The SCXI-1341 Lab-NB, Lab-PC, or Lab-PC+ cable assembly connects a Lab-NB, Lab-PC, or Lab-PC+ board to an SCXI-1121 module. The SCXI-1344 Lab-LC cable assembly connects a Lab-LC board to an SCXI-1121 module. The SCXI-1341 and SCXI-1344 cable assemblies consist of two pieces—an adapter board and a 50-conductor ribbon cable that connects the Lab board to the rear connector of the adapter board. The adapter board converts the signals from the Lab board I/O connectors to a format compatible with the SCXI-1121 rear signal connector pinout at the front connector of the SCXI-1341 or SCXI-1344. The adapter board also has an additional male breakout connector that makes the unmodified Lab board signals accessible to an SCXI-1180 feedthrough panel or an SCXI-1181 breadboard module. The adapter board gives the Lab boards full access to the digital control lines and analog signals, but the Lab boards cannot scan channels in Multiplexed mode. Leave jumper W1 in position A on the SCXI-1341 and SCXI-1344. The SCXI-1121 does not use jumper W1. Table E-2 lists the SCXI-1341 and SCXI-1344 pin translations.

Note: If you are using the Lab-PC+, configure the board for single-ended inputs.

Table E-2. SCXI-1341 and SCXI-1344 Pin Translations

Lab Board Pin	Lab Board Signal	SCXI-1121 Pin	SCXI-1121 Signal
1	ACH0	3	MCH0+
2	ACH1	5	MCH1+
3	ACH2	7	MCH2+
4	ACH3	9	MCH3+
5	ACH4	11	MCH4+
6	ACH5	13	No Connect
7	ACH6	15	No Connect
8	ACH7	17	No Connect
9	AIGND	1-2	AOGND
10	DAC0OUT	20	No Connect
11	AOGND	23	No Connect
12	DAC1OUT	21	No Connect
13, 50	DGND	24, 33	DIG GND
26	PB4	25	SERDATIN
27	PB5	27	DAQD*/A
28	PB6	29	SLOT0SEL*
29	PB7	37	SERCLK
31	PC1	26	SERDATOUT
32	PC2	28	No Connect
40	EXTCONV*	36	SCANCLK
43	OUTB1	46	No Connect
49	+5 V	34-35	No Connect

All other pins of the Lab board pinout are not sent to the SCXI-1121 rear signal connector.

SCXI-1341 and SCXI-1344 Installation

Follow these steps to install the SCXI-1341 or SCXI-1344:

1. Make sure that the computer and the SCXI chassis are turned off.
2. Install the SCXI module in the chassis.
3. Connect one end of the ribbon cable to the adapter board rear connector. This is the 50-pin connector of the SCXI-1344 cable.
4. Plug the adapter board front connector to the module rear signal connector. Make sure a corner of the adapter board enters the upper board guide of the chassis.
5. Screw the rear panel to the threaded strips in the rear of the chassis.
6. For an SCXI-1341, connect the loose end of the ribbon cable to the Lab-NB, Lab-PC, or Lab-PC+ I/O connector. For an SCXI-1344, connect the two 26-pin connectors to the Lab-LC according to the instructions given in the *Installation* section of Chapter 2, *Configuration and Installation*, of the *Lab-LC User Manual*.

Check the installation.

SCXI-1342 PC-LPM-16 Cable Assembly

The SCXI-1342 PC-LPM-16 cable assembly connects a PC-LPM-16 board to an SCXI-1121 module. The SCXI-1342 cable assembly consists of two pieces—an adapter board and a 50-conductor ribbon cable that connects the PC-LPM-16 board to the adapter board. The adapter board converts the signals from the PC-LPM-16 I/O connector to a format compatible with the SCXI-1121 rear signal connector pinout. The adapter board also has an additional male breakout connector that makes the unmodified PC-LPM-16 signals accessible to an SCXI-1180 feedthrough panel or an SCXI-1181 breadboard module. The adapter board gives the PC-LPM-16 full access to the digital control lines and analog signals, but the PC-LPM-16 cannot scan channels in Multiplexed mode. Leave jumper W1 in position A on the SCXI-1342. The SCXI-1121 does not use jumper W1. Table E-3 lists the SCXI-1342 pin translations.

Table E-3. SCXI-1342 Pin Translations

PC-LPM-16 Pin	PC-LPM-16 Signal	Rear Signal Connector Pin	SCXI-1121 Use
1-2	AIGND	1-2	AOGND
3	ACH0	3	MCH0+
4	ACH8	4	MCH0-
5	ACH1	5	MCH1+
6	ACH9	6	MCH1-
7	ACH2	7	MCH2+
8	ACH10	8	MCH2-
9	ACH3	9	MCH3+
10	ACH11	10	MCH3-
11	ACH4	11	MCH4+
12	ACH12	12	MCH4-
13	ACH5	13	No Connect
14	ACH13	14	No Connect
15	ACH6	15	No Connect
16	ACH14	16	No Connect
17	ACH7	17	No Connect
18	ACH15	18	No Connect
19, 50	DGND	24, 33	DIG GND
28	DIN6	26	SERDATOUT
29	DIN7	28	No Connect
34	DOUT4	25	SERDATIN
35	DOUT5	27	DAQD*/A
36	DOUT6	29	SLOT0SEL*
37	DOUT7	37	SERCLK
46	OUT2	46	No Connect
49	+5 V	34-35	No Connect

All other pins of the PC-LPM-16 pinout are not sent to the SCXI-1121 rear signal connector.

SCXI-1342 Installation

Follow these steps to install the SCXI-1342.

1. Make sure that the computer and the SCXI chassis are turned off.
2. Install the SCXI module to which the SCXI-1342 will connect.
3. Connect one end of the ribbon cable to the adapter board rear connector.
4. Plug the adapter board front connector onto the module rear signal connector. Make sure a corner of the adapter board enters the upper board guide of the chassis.
5. Screw the rear panel to the threaded strips in the rear of the chassis.
6. Connect the loose end of the ribbon cable to the PC-LPM-16 I/O connector.

Check the installation.

SCXI-1180 Feedthrough Panel

The SCXI-1180 feedthrough panel provides front-panel access to the signals of any data acquisition board that uses a 50-pin I/O connector. The SCXI-1180 consists of a front panel with a 50-pin male front panel connector that occupies one slot in the SCXI chassis, and a ribbon cable with a female rear connector and a male breakout connector. You can attach the rear connector to the male breakout connector of an SCXI-1340, SCXI-1341, SCXI-1342, SCXI-1344, or SCXI-1351 in the adjacent slot. The breakout connector further extends the cabling scheme. The front panel connector provides the feedthrough connection. You can attach an SCXI-1302 terminal block to the front panel connector for simple screw terminal connections. A rear filler panel that shields and protects the interior of the SCXI chassis is also included.

SCXI-1180 Installation

Install the SCXI-1180 to the right of a slot that has an SCXI-1340, SCXI-1341, SCXI-1342, or SCXI-1344 cable assembly or an SCXI-1351 slot extender in its rear connector space.

Follow these steps to install the SCXI-1180:

1. Make sure that the computer and the SCXI chassis are turned off.
2. Remove the front filler panel of the slot where you will insert the SCXI-1180.
3. Thread the rear connector through the front of the chassis to the rear of the chassis. Attach the rear connector to the breakout connector of the adjacent cable assembly or slot extender, as shown in Figure E-2.

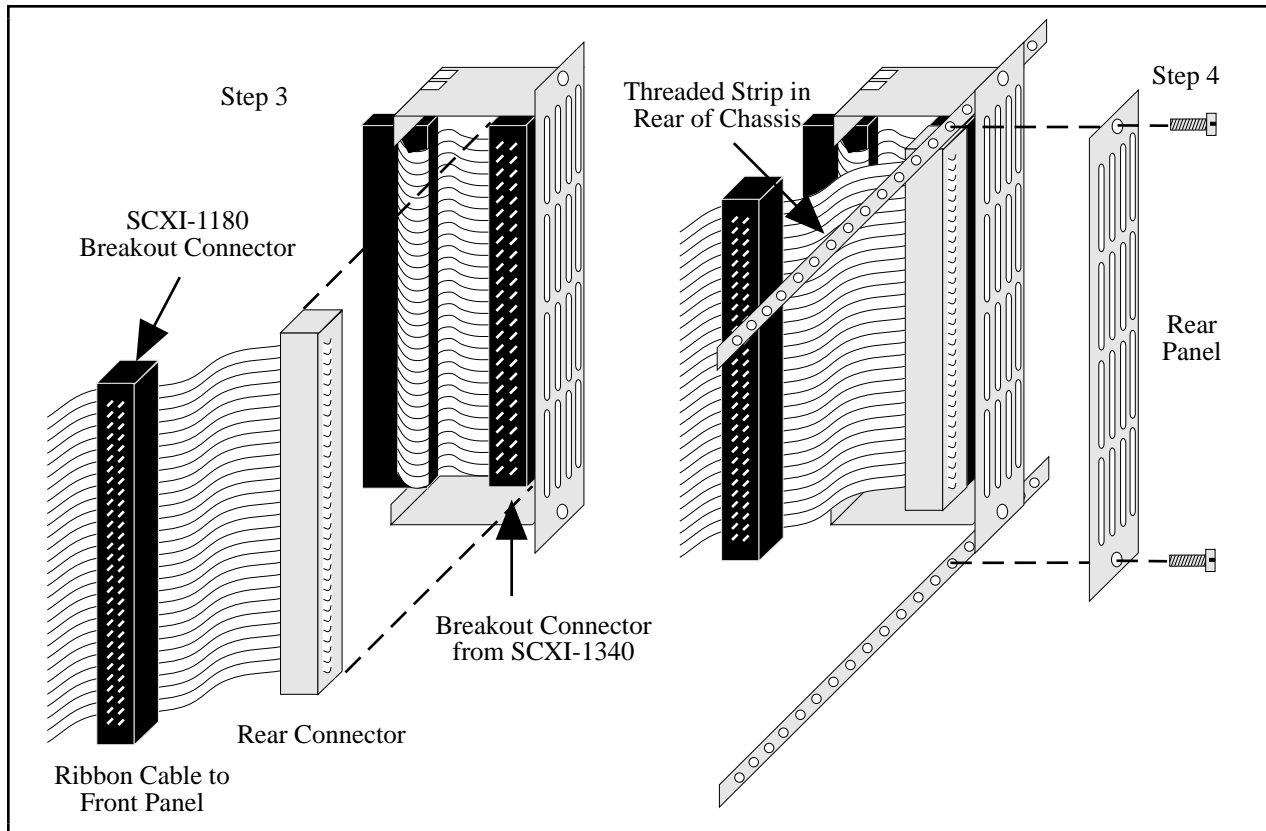


Figure E-2. SCXI-1180 Rear Connections

4. Screw in the rear panel to the threaded strip in the rear of the chassis.
5. Screw the front panel into the front threaded strip, as shown in Figure E-3.

Check the installation.

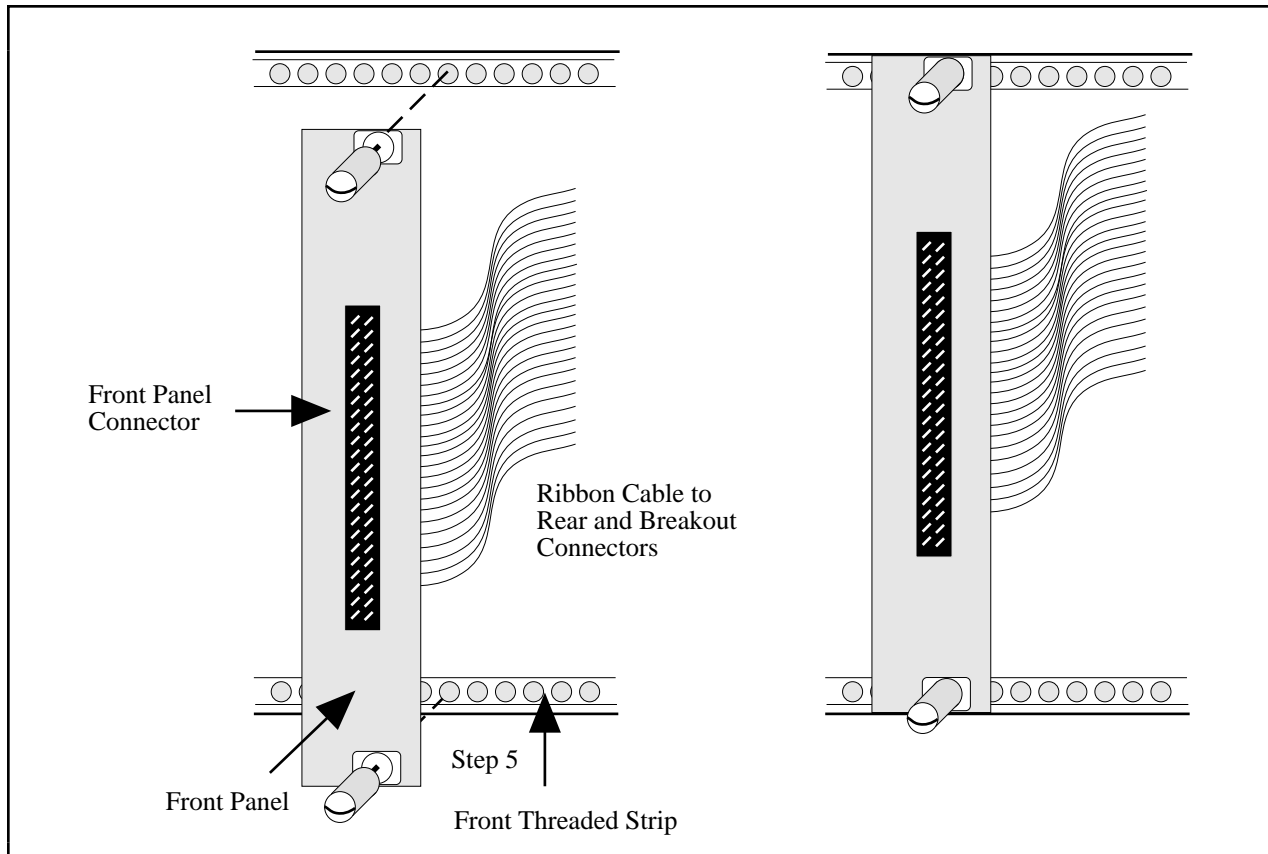


Figure E-3. SCXI-1180 Front Panel Installation

SCXI-1302 50-Pin Terminal Block

The SCXI-1302 terminal block has screw terminal connections for the 50-pin connector on the SCXI-1180 feedthrough panel.

SCXI-1302 Wiring Procedure

To wire the SCXI-1302 terminal block, you must remove the cover, connect all the wiring, and replace the cover. The procedure for this is as follows:

1. Unscrew the rear grounding screw on the back of the terminal block, as shown in Figure E-4.
2. With a flathead screwdriver, carefully pry the cover off the terminal block.
3. Insert each wire through the terminal block strain-relief opening.
4. Connect the wires to the screw terminals.
5. Tighten the large strain-relief screws to secure the wires.
6. Snap the cover back in place.
7. Reinsert the rear grounding screw. The terminal block is now ready to be connected to the front panel connector.

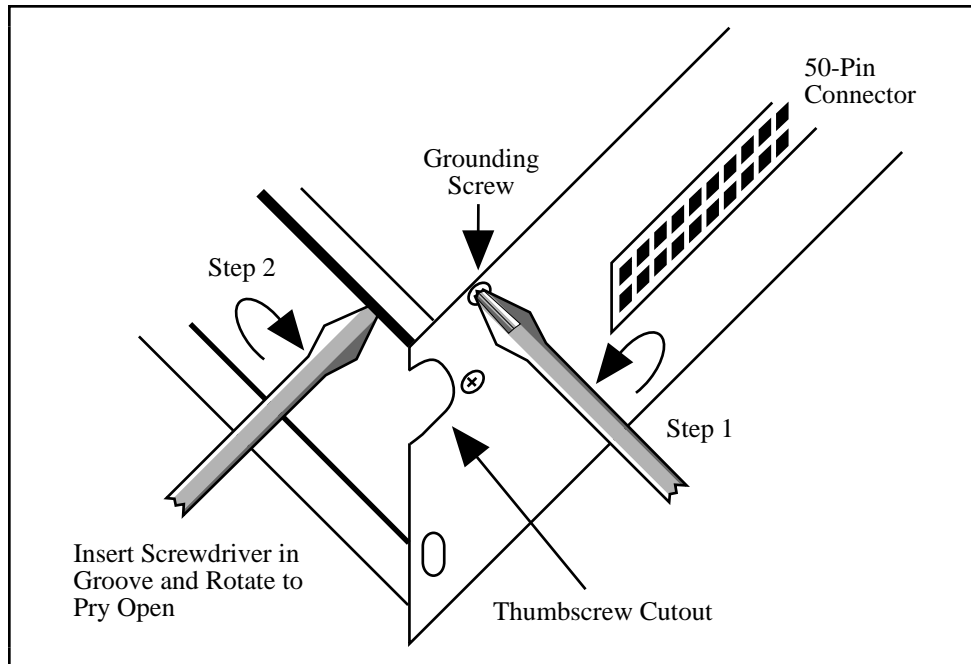


Figure E-4. Cover Removal

SCXI-1302 Installation

Follow these steps to install the SCXI-1302:

1. Install an SCXI-1180 feedthrough panel as described in the *SCXI-1180 Installation* section.
2. Wire the terminal block as described in the *SCXI-1302 Wiring Procedure* section.
3. Connect the SCXI-1302 terminal block to the front panel connector on the SCXI-1180 feedthrough panel. Be careful to fit the thumbscrews in the thumbscrew cutouts.
4. Tighten the top and bottom captive screws on the back of the terminal block into the screw holes in the front panel. This will hold the SCXI-1302 securely in place.
5. Check the installation.

SCXI-1351 One-Slot Cable Extender

The SCXI-1351 cable extender is a miniature SCXI-1340 cable assembly. Instead of connecting to an MIO board 1 m away, the SCXI-1351 female rear connector connects to the male breakout connector of a module that must be in the rear connector space of the slot to the left. The SCXI-1351 has a female mounting bracket connector that mates with the rear signal connector of a module, and also has a male breakout connector on the ribbon cable for connecting to a feedthrough panel or more cable extenders.

SCXI-1351 Installation

Follow these steps to install the SCXI-1351.

1. Make sure that the computer and the SCXI chassis are turned off.
2. Install the SCXI module in the chassis.
3. Connect the rear connector of the cable extender to the breakout connector in the adjacent slot. This attachment is similar to Step 3 in the *SCXI-1180 Installation* section, as shown in Figure E-2.
4. Plug the mounting bracket connector to the module rear signal connector. Make sure the alignment tab on the bracket enters the upper board guide of the chassis.
5. Screw the mounting bracket to the threaded strips in the rear of the chassis.

Check the installation.

SCXI-1350 Multichassis Adapter

You use the SCXI-1350 multichassis adapter to connect an additional SCXI-1001 chassis to the MIO-16 board. Using several SCXI-1350s, you can connect up to eight chassis to a single MIO board. The SCXI-1350 consists of a multichassis adapter board. You will also need a ribbon cable for each chassis-to-chassis connection, as well as a ribbon cable to connect the MIO board to the first chassis.

Note: Use 0.5 m ribbon cable when connecting multiple chassis together to minimize cable length and maintain signal integrity. You can use a 1 m cable to connect the MIO board to the first chassis.

The adapter board has a male rear connector, a female front connector, and a male chassis extender connector. You can attach the rear connector to a ribbon cable from the MIO board or a preceding chassis. You connect the front connector with the module rear signal connector. You connect the chassis extender connector to a ribbon cable that goes to the subsequent chassis. The adapter takes Channel 0 from the front connector and sends it to Channel 0 of the rear connector. The adapter also takes channels 0 through 6 on the chassis extender connector and maps them to channels 1 through 7, respectively, on the rear connector.

SCXI-1350 Installation

Follow these steps to install the SCXI-1350:

1. Make sure that the computer and all the SCXI chassis are turned off.
2. Insert all the modules in all the chassis.
3. Connect one end of a ribbon cable to the MIO board.
4. Connect the other end of the ribbon cable to the rear connector of the first SCXI-1350.

5. Connect another ribbon cable or cable assembly to the chassis extender connector.
6. Plug the adapter board front connector to the module rear signal connector. Make sure a corner of the adapter board enters the upper board guide of the chassis.
7. Screw the rear panel to the threaded strips in the rear of the chassis.
8. Connect the cable assembly to the desired module in the second chassis, or if you are using more than two chassis, connect the loose end of the ribbon cable to the rear connector of the second SCXI-1350, and install the adapter board.
9. Continue until all chassis are connected. For N chassis, you will need N ribbon cables and N multichassis adapters.

SCXI-1343 Rear Screw Terminal Adapter

You use the SCXI-1343 universal adapter to adapt custom wiring to the SCXI-1121. The SCXI-1343 has screw terminals for the analog output connections and solder pads for the rest of the signals. A strain-relief clamp is on the outside of the rear panel. Table E-4 shows the SCXI-1343 pin connections.

SCXI-1343 Installation

1. Insert each wire through the adapter strain-relief opening.
2. Make all solder connections first.
3. Connect the other wires to the screw terminals.
4. Tighten the strain-relief screws to secure the wires.
5. Plug the adapter board front connector to the module rear signal connector. Make sure a corner of the adapter board enters the upper board guide of the chassis.
6. Screw the rear panel to the threaded strips in the rear of the chassis.

Table E-4. SCXI-1343 Pin Connections

Rear Signal Connector Pin	SCXI-1121 Use	Connection Type
1	AOGND	Solder pad
2	AOGND	Screw terminal
3	MCH0+	Screw terminal
4	MCH0-	Screw terminal
5	MCH1+	Screw terminal
6	MCH1-	Screw terminal
7	MCH2+	Screw terminal
8	MCH2-	Screw terminal
9	MCH3+	Screw terminal
10	MCH3-	Screw terminal
11	MCH4+	Screw terminal
12	MCH4-	Screw terminal
13	No Connect	Screw terminal
14	No Connect	Screw terminal
15	No Connect	Screw terminal
16	No Connect	Screw terminal
17	No Connect	Screw terminal
18	No Connect	Screw terminal
19	OUTREF	Screw terminal
20	No Connect	Solder pad
21	No Connect	Solder pad
22	No Connect	Solder pad
23	No Connect	Solder pad
24, 33	DIG GND	Solder pad
26	SERDATOUT	Solder pad
27	DAQD*/A	Solder pad
28	No Connect	Solder pad
29	SLOT0SEL*	Solder pad
30	No Connect	Solder pad
31	No Connect	Solder pad
32	No Connect	Solder pad
33	No Connect	Solder pad
34-35	No Connect	Solder pad
36	SCANCLK	Solder pad
37	SERCLK	Solder pad
38	No Connect	Solder pad
39	No Connect	Solder pad
40	No Connect	Solder pad
41	No Connect	Solder pad
42	No Connect	Solder pad
43	RSVD	Solder pad
44	No Connect	Solder pad
45	No Connect	Solder pad
46	No Connect	Solder pad
47	No Connect	Solder pad
48	No Connect	Solder pad
49	No Connect	Solder pad
50	No Connect	Solder pad

Appendix F

Revision A and B Photo and Parts Locator Diagrams

This appendix contains a photograph of the Revision A and B SCXI-1121 signal conditioning module and the general and detailed parts locator diagrams.

Figure F-1 shows the SCXI-1121 module. Figures F-2 and F-3 show the general and detailed parts locator diagrams of the Revision A and B SCXI-1121.



Figure F-1. Revision A and B SCXI-1121 Signal Conditioning Module




Figure F-2. Revision A and B SCXI-1121 General Parts Locator Diagram




Figure F-3. Revision A and B SCXI-1121 Detailed Parts Locator Diagram

Appendix G

Customer Communication

For your convenience, this appendix contains forms to help you gather the information necessary to help us solve technical problems you might have as well as a form you can use to comment on the product documentation. Filling out a copy of the *Technical Support Form* before contacting National Instruments helps us help you better and faster.

National Instruments provides comprehensive technical assistance around the world. In the U.S. and Canada, applications engineers are available Monday through Friday from 8:00 a.m. to 6:00 p.m. (central time). In other countries, contact the nearest branch office. You may fax questions to us at any time.

Corporate Headquarters

(512) 795-8248

Technical support fax: (800) 328-2203

(512) 794-5678

Branch Offices	Phone Number	Fax Number
Australia	(03) 879 9422	(03) 879 9179
Austria	(0662) 435986	(0662) 437010-19
Belgium	02/757.00.20	02/757.03.11
Denmark	45 76 26 00	45 76 71 11
Finland	(90) 527 2321	(90) 502 2930
France	(1) 48 14 24 00	(1) 48 14 24 14
Germany	089/741 31 30	089/714 60 35
Italy	02/48301892	02/48301915
Japan	(03) 3788-1921	(03) 3788-1923
Netherlands	03480-33466	03480-30673
Norway	32-848400	32-848600
Spain	(91) 640 0085	(91) 640 0533
Sweden	08-730 49 70	08-730 43 70
Switzerland	056/27 00 20	056/27 00 25
U.K.	0635 523545	0635 523154

Technical Support Form

Photocopy this form and update it each time you make changes to your software or hardware, and use the completed copy of this form as a reference for your current configuration. Completing this form accurately before contacting National Instruments for technical support helps our applications engineers answer your questions more efficiently.

If you are using any National Instruments hardware or software products related to this problem, include the configuration forms from their user manuals. Include additional pages if necessary.

Name _____

Company _____

Address _____

Fax (____) _____ Phone (____) _____

Computer brand _____ Model _____ Processor _____

Operating system _____

Speed _____ MHz RAM _____ MB Display adapter _____

Mouse _____ yes _____ no Other adapters installed _____

Hard disk capacity _____ MB Brand _____

Instruments used _____

National Instruments hardware product model _____ Revision _____

Configuration _____

National Instruments software product _____ Version _____

Configuration _____

The problem is _____

List any error messages _____

The following steps will reproduce the problem _____

SCXI-1121 Hardware Configuration Form

Record the settings and revisions of your hardware and software on the line to the right of each item. Complete a new copy of this form each time you revise your software or hardware configuration, and use this form as a reference for your current configuration. Completing this form accurately before contacting National Instruments for technical support helps our applications engineers answer your questions more efficiently.

- SCXI-1121 Revision Letter _____
- Chassis Slot _____
- Grounding, Shielding, and Reference Mode Selection (Factory Setting: Parking position, W33, A-R0R1) _____
- Half-Bridge Completion Network (Factory Setting Disabled)
 - Channel 0 _____
 - Channel 1 _____
 - Channel 2 _____
 - Channel 3 _____

- Input Channel Configuration

Input Channel	First Stage Gain	Second Stage Gain	Total Gain	Filter
Factory Setting	A = 100	D = 10	1,000	4 Hz
0				
1				
2				
3				

- Excitation Channel Configuration

Excitation Channel	Mode	Level
Factory Setting	Voltage	3.333 V
0		
1		
2		
3		

- Other Modules in System _____

- Data Acquisition Boards Installed _____

Documentation Comment Form

National Instruments encourages you to comment on the documentation supplied with our products. This information helps us provide quality products to meet your needs.

Title: **SCXI-1121 User Manual**

Edition Date: **August 1994**

Part Number: **320426B-01**

Please comment on the completeness, clarity, and organization of the manual.

If you find errors in the manual, please record the page numbers and describe the errors.

Thank you for your help.

Name _____

Title _____

Company _____

Address _____

Phone (_____) _____

Mail to: Technical Publications
National Instruments Corporation
6504 Bridge Point Parkway, MS 53-02
Austin, TX 78730-5039

Fax to: Technical Publications
National Instruments Corporation
MS 53-02
(512) 794-5678

Glossary

Prefix	Meaning	Value
p-	pico-	10 ⁻¹²
n-	nano-	10 ⁻⁹
μ-	micro-	10 ⁻⁶
m-	milli-	10 ⁻³
k-	kilo-	10 ³
M-	mega-	10 ⁶

Numbers/Symbols

°	degrees
Ω	ohms
ε	strain
+5 V (signal)	+5 VDC Source signal

A

A	amperes
AB0+	Positive Analog Bus 0 Line signal
AB0-	Negative Analog Bus 0 Line signal
AB0EN	Analog Bus 0 Enable bit
AB2+	Positive Analog Bus 2 Line signal
AB2-	Negative Analog Bus 2 Line signal
ACH#	data acquisition board Analog Input Channel Number
A/D	analog-to-digital
AOGND	Analog Output Ground signal
Arms	amperes, root mean square
AWG	American Wire Gauge

B

BW	bandwidth
----	-----------

C

C	Celsius
CH#+	Positive Input Channel Number signal
CH#-	Negative Input Channel Number signal
CHAN	Channel Select bit
CHS	Chassis bit
CHSGND	Chassis Ground signal
CJR	cold-junction reference
CLKEN	Clock Enable bit

CLKOUTEN	Scanlock Output Enable bit
CLKSELECT	Scanlock Select bit
CNT	Count bit

D

D*/A	Data/Address Line signal
D/A	digital-to-analog
DAQD*/A	Data Acquisition Board Data/Address Line signal
dB	decibels
DIG GND	Digital Ground signal
DIN	Deutsche Industrie Norme
DMM	digital multimeter
DTEMP	Direct Temperature Sensor
DTS	direct temperature sensor

E

EGND#	Excitation Ground Number signal
EX#+	Positive Excitation Output Number signal
EX#-	Negative Excitation Output Number signal

F

F	Fahrenheit
FIFO	first-in-first-out
FOUTEN*	Forced Output Enable bit
FRT	Forced Retransmit bit

G

GBWP	gain bandwidth product
GUARD	Guard signal

H

hex	hexadecimal
HSCR	Hardscan Control Register
HSRS*	Hardscan Reset bit
Hz	hertz

I

I_l	input current leakage
in.	inches
INTR*	Interrupt signal
I/O	input/output

K

K kelvin

L

LOAD* Load bit
LSB least significant bit

M

m meters
M megabytes of memory
MCH#+ Positive Analog Output Channel Number signal
MCH#- Negative Analog Output Channel Number signal
MISO Master-In Slave-Out signal
MOD Module Number bit
MOSI Master-Out Slave-In signal
MSB most significant bit
MTEMP Multiplexed Temperature Sensor
MTS multiplexed temperature sensor

N

NRSE nonreferenced single-ended (input)

O

ONCE Once bit
OUTREF Output Reference signal

P

ppm parts per million

R

RAM random-access memory
RD Read bit
RESET* Reset signal
rms root mean square
RSE referenced single-ended (input)
RSVD Reserved bit/signal
RTD resistance temperature detector
RTEMP Read Temperature bit
RTI Referred To Input
RTO Referred To Output
RTSI Real Time System Integration

S

SCAL (bit)	Shunt Calibrate bit
SCAL (signal)	Shunt Calibration signal
SCANCLK	Scan Clock signal
SCANCLKEN	Scan CLock Enable bit
SCANCON	Scanning Control signal
SCANCONEN	Scan Control Enable bit
SCANCONEN	Scan Control Enable bit
SCXI	Signal Conditioning eXtensions for Instrumentation (bus)
SDK	Software Developer's Kit
sec	seconds
SERCLK	Serial Clock signal
SERDATIN	Serial Data In signal
SERDATOUT	Serial Data Out signal
SL	Slot bit
SLOT0SEL*	Slot 0 Select signal
SPI	serial peripheral interface
SPICLK	Serial Peripheral Interface Clock signal
SS*	Slot Select signal

T

tempco	temperature coefficient
TRIG0	Trigger 0 signal

U

UL	Underwriters Laboratory
----	-------------------------

V

V	volts
V+	Positive Analog Supply signal
V-	Negative Analog Supply signal
VDC	volts direct current
V _{IH}	volts input high
V _{IL}	volts input low
V _{OH}	volts output high
V _{OL}	volts output low
V _{rms}	volts, root mean square

W

W	watts
---	-------

Index

Numbers/Symbols

- +5 V signal
 - front connector, 2-15, D-2
 - SCXIbus connector, 3-4, C-3

A

- AB0- signal, 3-4, C-3
- AB0+ signal, 3-4, C-3
- AB0EN bit, 4-4
- AC-coupled signal connection, 2-18
- analog and timing circuitry, 3-8 to 3-15
 - analog input channels, 3-8 to 3-10
 - analog input block diagram, 3-9
 - analog output circuitry, 3-14 to 3-15
 - calibration, 3-11 to 3-13
 - equipment requirements, 3-11
 - excitation adjust, 3-12 to 3-13
 - offset null adjust, 3-12
 - potentiometers reference designators, 3-13
 - excitation output channels, 3-10
- analog configuration, 2-7 to 2-12
 - excitation jumpers, 2-10 to 2-12
 - current and voltage excitation jumpers, 2-10
 - excitation level, 2-10 to 2-11
 - internal half-bridge completion, 2-11 to 2-12
- grounding, shielding, and reference mode selection (jumper W33), 2-7 to 2-8
- input channel jumpers
 - filter jumpers, 2-9
 - gain jumpers, 2-8 to 2-9
- analog input channels, 2-17 to 2-19
 - AC-coupled signal connection, 2-18
 - analog input block diagram, 3-9
 - floating AC-coupled signal connection, 2-18
 - floating signal connection, 2-17
 - ground-referenced signal connection, 2-17
 - theory of operation, 3-8 to 3-10
 - warning against exceeding input range, 2-19
- analog input specifications, A-1 to A-2

- analog output circuitry, 3-14 to 3-15
- analog output signal connections, 2-35
- AOGND signal
 - jumper connection, 2-8
 - rear signal connector, 2-34, B-2

B

- bit descriptions
 - AB0EN, 4-4
 - CHAN<1..0>, 4-3
 - CHS<4..0>, 4-6
 - CLKEN, 4-7
 - CLKOUTEN, 4-3
 - CLKSELECT, 4-3
 - CNT<6..0>, 4-8
 - FOUTEN*, 4-4
 - FRT, 4-7
 - HSRS*, 4-7
 - LOAD*, 4-7
 - MOD<3..0>, 4-8
 - ONCE, 4-7
 - RD, 4-7
 - RSVD, 4-4, 4-7
 - RTEMP, 4-4
 - SCAL, 4-3
 - SCANCLKEN, 4-4
 - SCANCONEN, 4-4, 4-7
 - SL<3..0>, 4-6
- board configuration. *See* configuration.

C

- cabling
 - custom cables, 1-3 to 1-4
 - SCXI-1180 feedthrough panel
 - cable assembly, E-6
 - front panel installation, E-8
 - installation, E-6 to E-8
 - rear connections, E-7
 - SCXI-1302 50-pin terminal block
 - cover removal, E-9
 - installation, E-9
 - wiring procedure, E-8
 - SCXI-1340
 - cable assembly, E-1 to E-2
 - installation, E-2 to E-3
 - SCXI-1341

- cable assembly, E-3 to E-4
 - installation, E-4
 - pin translations, E-4
- SCXI-1342
 - cable assembly, E-5
 - installation, E-6
 - pin translations, E-5
- SCXI-1343 rear screw terminal adapter
 - cable assembly, E-11
 - installation, E-11
 - pin connections, E-12
- SCXI-1344
 - cable assembly, E-3 to E-4
 - installation, E-4
 - pin translations, E-4
- SCXI-1350 multichassis adapter
 - cable assembly, E-10
 - installation, E-10 to E-11
- SCXI-1351 one-slot cable extender
 - cable assembly, E-9
 - installation, E-10
- calibration, 3-11 to 3-13
 - equipment requirements, 3-11
 - excitation adjust, 3-12 to 3-13
 - offset null adjust, 3-12
 - potentiometers reference designators, 3-13
- CGND signal
 - front connector, 2-15, D-2
- CHSGND signal
 - SCXIBus connector, 3-4, C-3
- CH0- signal, 2-16, D-3
- CH0+ signal, 2-16, D-3
- CH1- signal, 2-16, D-3
- CH1+ signal, 2-16, D-3
- CH2- signal, 2-16, D-3
- CH2+ signal, 2-16, D-3
- CH3- signal, 2-15, D-2
- CH3+ signal, 2-15, D-2
- CHAN<1..0> bit, 4-3
- channel scanning. *See* scanning measurements.
- CHS<4..0> bit, 4-6
- CLKEN bit, 4-7
- CLKOUTEN bit, 4-3
- CLKSELECT bit, 4-3
- CNT<6..0> bit, 4-8
- cold-junction sensor specifications, A-3
- communication signals
 - communicating on SPI bus, 2-37 to 2-40
 - Configuration Register write timing diagram, 2-40
 - Module ID Register timing diagram, 2-40
 - reading from Module ID Register, 2-40
 - serial data timing diagram, 2-39
 - slot-select timing diagram, 2-38
 - slot-selection procedure, 2-38 to 2-39
 - writing to Configuration Register, 2-39 to 2-40
- configuration. *See also* signal connections
 - analog configuration, 2-7 to 2-12
 - excitation jumpers, 2-10 to 2-12
 - current and voltage excitation jumpers, 2-10
 - excitation level, 2-10 to 2-11
 - internal half-bridge completion, 2-11 to 2-12
 - grounding, shielding, and reference mode selection (jumper W33), 2-7 to 2-8
 - input channel jumpers
 - filter jumpers, 2-9
 - gain jumpers, 2-8 to 2-9
 - digital signal connections, 2-4 to 2-7
 - jumper W32, 2-5 to 2-7
 - jumper W38, 2-5 to 2-6
 - jumper W44, 2-5, 2-6
 - fixed jumpers, 2-4
 - parts locator diagram
 - detailed, 2-3
 - general, 2-2
- SCXI-1320 terminal block, 2-21, 2-26 to 2-29, 2-32
 - installation, 2-32
 - jumper configuration, 2-27
 - parts locator diagram, 2-29
 - signal connection, 2-28
 - specifications, A-3
 - temperature sensor, 2-26
- SCXI-1321 offset-null and shunt-calibration terminal block, 2-21 to 2-28, 2-31 to 2-32
 - installation, 2-32
 - jumper configuration, 2-27 to 2-28
 - nulling circuitry, 2-21 to 2-22
 - parts locator diagram, 2-31
 - shunt calibration, 2-24 to 2-25
 - signal connection, 2-28
 - specifications, A-3
 - temperature sensor, 2-26
 - using with RTDs and thermistors, 2-23 to 2-24
- SCXI-1328 high-accuracy isothermal terminal block, 2-21, 2-26 to 2-28, 2-30, 2-32
 - installation, 2-32
 - jumper configuration, 2-27

- parts locator diagram, 2-30
- signal connection, 2-28
- specifications, A-3
- temperature sensor, 2-26
- SCXI-1330 connector-and-shell assembly, 2-19 to 2-20
- user-configurable jumpers, 2-4
- Configuration Register
 - description of, 4-3 to 4-4
 - digital control circuitry, 3-7 to 3-8
 - write procedure, 2-39 to 2-40
 - write timing diagram, 2-40
- connector-and-shell assembly. *See* SCXI 1330 connector-and-shell assembly.
- Counter 1 and SCANDIV, 5-8
- Current excitation mode, 2-10
- customer communication, *xiii*, G-1

D

- D*/A signal, 3-4, C-3
- DAQD*/A signal
 - communicating on SPI bus, 2-37 to 2-40
 - digital I/O signal connections, 2-35 to 2-37
 - reading from Module ID Register, 2-40
 - rear signal connector, 2-34, B-2
 - register selection and write procedure, 5-2
 - writing the slot-select number, 2-38
 - writing to Configuration Register, 2-39
- data acquisition board setup programming, 5-6 to 5-8
 - Counter 1 and SCANDIV, 5-8
- DIG GND signal, 2-34, B-2
- digital control circuitry, 3-7 to 3-8
- digital I/O signal connections
 - rear signal connector, 2-35 to 2-37
 - SCXIbus pin equivalences with SCXI 1121 and data acquisition boards, 2-36
- digital interface, 3-6
- digital signal connections, 2-4 to 2-7
 - jumper W32, 2-5 to 2-7
 - jumper W38, 2-5 to 2-6
 - jumper W44, 2-5 to 2-6
- direct measurements. *See* single-channel measurements.
- documentation
 - conventions used in manual, *xii*
 - organization of manual, *xi-xii*

- related documentation, *xiii*
- DTEMP signal, 2-15, D-2

E

- EGND0 signal, 2-16, D-3
- EGND1 signal, 2-16, D-3
- EGND2 signal, 2-15, D-2
- EGND3 signal, 2-15, D-2
- equipment, optional, 1-3
- EX0- signal, 2-16, D-3
- EX0+ signal, 2-16, D-3
- EX1- signal, 2-16, D-3
- EX1+ signal, 2-16, D-3
- EX2- signal, 2-16, D-3
- EX2+ signal, 2-16, D-3
- EX3- signal, 2-15, D-2
- EX3+ signal, 2-15, D-2
- excitation channels
 - calibration, 3-12 to 3-13
 - front connector, 2-19
 - maximum load per channel, 2-10
 - theory of operation, 3-10
- excitation jumpers, 2-10 to 2-12
 - current and voltage excitation jumpers, 2-10
 - excitation level, 2-10 to 2-11
 - internal half-bridge completion, 2-11 to 2-12

F

- fax technical support, G-1
- FIFO Register, 4-8
- filter jumpers, 2-9
- fixed jumpers, 2-4
- floating AC-coupled signal connection, 2-18
- floating signal connection, 2-17
- FOUTEN* bit, 4-4
- front connector
 - analog input channels, 2-17 to 2-19
 - AC-coupled signal connection, 2-18
 - floating AC-coupled signal connection, 2-18
 - floating signal connection, 2-17
 - ground-referenced signal connection, 2-17
 - warning against exceeding input range, 2-19
 - excitation channels, 2-19
 - pin assignments, 2-14, D-1

signal descriptions, 2-15 to 2-17,
D-2 to D-3
temperature sensor connection, 2-19
FRT bit, 4-7
functional overview. *See* theory of
operation.

G

gain jumpers, 2-8 to 2-9
ground-referenced signal connection, 2-17
grounding, shielding, and reference mode
selection (jumper W33), 2-7 to 2-8
GUARD signal, 3-4, C-3

H

half-bridge completion, internal,
2-11 to 2-12
hardscan circuitry, programming,
5-11 to 5-12
Hardscan Control Register, 4-7
hardware installation, 2-12 to 2-13
HSRS* bit, 4-7

I

indirect measurements. *See* single-channel
measurements.
input channel jumpers
filter jumpers, 2-9
gain jumpers, 2-8 to 2-9
installation. *See also* cabling.
hardware installation, 2-12 to 2-13
SCXI-1180 feedthrough panel,
E-6 to E-8
SCXI-1302 50-pin terminal block, E-9
SCXI-1320 terminal block, 2-32
SCXI-1321 offset-null and shunt-
calibration terminal block, 2-32
SCXI-1328 high-accuracy isothermal
terminal block, 2-32
SCXI-1340, E-2 to E-3
SCXI-1341, E-4
SCXI-1342, E-6
SCXI-1343 rear screw terminal
adapter, E-11
SCXI-1344, E-4
SCXI-1350 multichassis adapter,
E-10 to E-11

SCXI-1351 one-slot cable
extender, E-10
unpacking the SCXI-1121, 1-4
internal half-bridge completion, 2-11 to 2-12
INTR* line and signal
jumper connection, 2-4, 2-5
SCXibus connector, 3-4, C-3

J

jumpers, analog configuration
excitation jumpers, 2-10 to 2-12
current and voltage excitation
jumpers, 2-10
excitation level, 2-10 to 2-11
internal half-bridge completion,
2-11 to 2-12
grounding, shielding, and reference mode
selection (jumper W33), 2-7 to 2-8
input channel jumpers
filter jumpers, 2-9
gain jumpers, 2-8 to 2-9
digital signal connections
jumper W32, 2-5 to 2-7
jumper W38, 2-5 to 2-6
jumper W44, 2-5
fixed jumpers, 2-4
nulling circuitry, 2-23 to 2-24
parts locator diagram
detailed, 2-3
general, 2-2
SCXI-1320 terminal block, 2-27
SCXI-1321 offset-null and shunt-
calibration terminal block,
2-27 to 2-28
SCXI-1328 high-accuracy isothermal
terminal block, 2-27
user-configurable jumpers, 2-4

L

Lab-LC. *See* SCXI-1344.
Lab-NB/Lab-PC/Lab-PC+. *See* SCXI-1341.
LabVIEW software, 1-2
LabWindows software, 1-2
LOAD* bit, 4-7

M

manual. *See* documentation.

MCH0± through MCH4± signal
 analog output circuitry, 3-15
 rear signal connector, 2-34, B-2
 measurements. *See* scanning measurements;
 single-channel measurements.
 MISO signal
 jumper connection, 2-4, 2-5, 2-6
 SCXIBus connector, 3-4, C-3
 MOD<3..0> bit, 4-8
 module configuration, 2-1
 fixed jumpers, 2-4
 user-configurable jumpers, 2-4
 Module ID Register
 description of, 4-2
 digital control circuitry, 3-8
 read procedure, 2-40
 timing diagram, 2-40
 module programming, 5-9 to 5-11
 channel scanning from other
 modules, 5-9
 channel scanning from SCXI-1121 via
 another module, 5-10
 multiple-chassis scanning, 5-11
 multiple-module multiplexed
 scanning, 5-10
 single-module multiplexed scanning, 5-9
 single-module parallel scanning, 5-9
 MOSI signal, 3-4, C-4
 MTEMP signal
 analog output circuitry, 3-15
 front connector, 2-15, 2-26, D-2
 multiplexed output
 analog output circuitry, 3-15
 single-channel measurements, 5-3 to 5-4
 Multiplexed-Output mode, 1-1
 multiplexed scanning, 3-16 to 3-18
 multiple-chassis scanning, 3-18, 5-11
 multiple-module multiplexed scanning,
 3-17 to 3-18, 5-10
 single-module multiplexed scanning,
 3-16 to 3-17
 direct, 3-16 to 3-17
 indirect, 3-17
 MUXCOUNTER
 analog output circuitry, 3-14
 incrementing, 2-36, 2-37
 multiplexed scanning, 3-16 to 3-17

N

NI-DAQ software, 1-2
 nulling circuitry, 2-21 to 2-23

jumper settings, 2-23 to 2-24
 nulling circuit, 2-23
 nulling offset voltage, 2-22 to 2-23
 nulling resistors and corresponding
 channel, 2-22
 strain formula for quarter-bridge strain
 gauge configuration, 2-23
 trimmer potentiometer and
 corresponding channel, 2-22

O

offset null adjust, 3-12
 ONCE bit, 4-7
 operating environment specifications, A-4
 operation of SCXI-1121. *See* theory of
 operation.
 OUTREF signal
 jumper connection, 2-7
 rear signal connector, 2-34, B-2

P

parallel output
 analog output circuitry, 3-15
 single-channel measurements, 5-3
 Parallel-Output mode, 1-1
 parallel scanning, single-module,
 3-15 to 3-16
 physical specifications, A-3
 pin assignments
 front connector, 2-14, D-1
 rear signal connector, 2-33, B-1
 SCXI-1343 rear screw terminal
 adapter, E-12
 SCXIBus connector, 3-3, C-2
 pin equivalences
 SCXI-1121 and MIO-16, E-2
 SCXI-1341/1344, E-4
 SCXI-1342, E-5
 SCXIBus connector
 rear signal connector, 3-5
 rear signal connector and data
 acquisition boards, 2-36, 5-2
 programming. *See also* registers.
 notation for bit patterns, 5-1
 register writes, 5-1 to 5-3
 initialization, 5-3
 register selection and write
 procedure, 5-2 to 5-3
 SCXI-1121 rear signal connector pin
 equivalences, 5-2

- scanning measurements, 5-6 to 5-15
 - acquisition enable, triggering, and servicing, 5-12
 - data acquisition board setup programming, 5-6 to 5-8
 - Counter 1 and SCANDIV, 5-8
 - module programming, 5-9 to 5-11
 - multiple-chassis scanning, 5-11
 - multiple-module multiplexed scanning, 5-10
 - single-module multiplexed scanning (direct), 5-9
 - single-module multiplexed scanning (indirect), 5-9
 - single-module parallel scanning, 5-9
 - scanning examples, 5-13 to 5-15
 - Slot 0 hardscan circuitry, 5-11 to 5-12
 - single-channel measurements, 5-3 to 5-5
 - direct measurements, 5-3 to 5-4
 - indirect measurements, 5-4 to 5-5
 - measurements from other modules, 5-4
 - measurements from SCXI-1121 via another module, 5-5
 - multiplexed output, 5-3 to 5-4
 - parallel output, 5-3
 - Pseudodifferential Reference mode, 2-7 to 2-8
- R**
- RD bit, 4-7
 - rear signal connector, 2-32 to 2-40
 - analog output signal connections, 2-35
 - communication protocol, 2-37
 - communication signals, 2-37 to 2-40
 - digital I/O signal connections, 2-35 to 2-37
 - pin assignments, 2-33, B-1
 - pin equivalences
 - with SCXIBus and data acquisition boards, 2-36, 5-2
 - with SCXIBus connector, 3-5
 - signal descriptions, 2-34 to 2-35, B-2
 - timing requirements, 2-37
 - reference mode selection (jumper W33), 2-7
 - registers
 - programming considerations
 - initialization, 5-3
 - register selection and write procedure, 5-2 to 5-3
 - register writes, 5-1 to 5-3
 - SCXI-1121 rear signal connector pin equivalences, 5-2
 - SCXI-1121 registers, 4-1 to 4-4
 - Configuration Register, 2-39 to 2-40, 3-7, 4-3 to 4-4
 - Module ID Register, 2-40, 3-8, 4-2
 - Slot 0 registers, 4-5 to 4-8
 - FIFO Register, 4-8
 - Hardscan Control Register, 4-7 overview, 4-5
 - Slot-Select Register, 4-6
 - RESET* signal, 3-4, C-3
 - Revision A and B SCXI-1121 signal conditioning module
 - detailed parts locator diagram, F-3
 - general parts locator diagram, F-2
 - photograph, F-1
 - RSVD bit, 4-4, 4-7
 - RSVD signal
 - front connector, 2-15, D-2
 - rear signal connector, 2-34, B-2
 - SCXIBus connector, 3-4, C-3
 - RTD mode specifications, A-2
 - RTDs, using with SCXI-1321, 2-23
 - RTEMP bit, 4-4
- S**
- SCAL bit, 4-3
 - SCAL signal, 2-15, D-2
 - SCANCLK signal
 - analog output circuitry, 3-14
 - multiplexed scanning, 3-16 to 3-17
 - rear signal connector, 2-34, B-2
 - timing requirements, 2-37
 - SCANCLKEN bit, 4-4
 - SCANCON signal
 - analog output circuitry, 3-14
 - multiplexed scanning, 3-16 to 3-17
 - SCXIBus connector, 3-4, C-4
 - SCANCONEN bit, 4-4, 4-7
 - SCANDIV bit, 5-8
 - scanning measurements, 5-6 to 5-15
 - acquisition enable, triggering, and servicing, 5-12
 - data acquisition board setup programming, 5-6 to 5-8
 - Counter 1 and SCANDIV, 5-8
 - module programming, 5-9 to 5-11
 - multiple-chassis scanning, 5-11
 - multiple-module multiplexed scanning, 5-10

- single-module multiplexed scanning (direct), 5-9
 - single-module multiplexed scanning (indirect), 5-9
 - single-module parallel scanning, 5-9
- scanning examples, 5-13 to 5-15
- Slot 0 hardscan circuitry, 5-11 to 5-12
- scanning modes
 - multiplexed scanning, 3-16 to 3-18
 - multiple-chassis scanning, 3-18
 - multiple-module multiplexed scanning, 3-17 to 3-18
 - single-module multiplexed scanning, 3-16 to 3-17
 - single-module parallel scanning, 3-15 to 3-16
- SCXI-1121. *See also* configuration; installation.
 - block diagram, 3-1
 - contents of kit, 1-1
 - custom cables, 1-3 to 1-4
 - definition of, 1-1
 - equipment, optional, 1-3
 - overview, 1-1 to 1-2
 - Revision A and B module
 - detailed parts locator diagram, F-3
 - general parts locator diagram, F-2
 - photograph, F-1
 - software, optional, 1-2
 - support for MIO-16 boards, 1-1
 - unpacking, 1-4
- SCXI-1121 registers, 4-1 to 4-4
 - Configuration Register
 - description of, 4-3 to 4-4
 - digital control circuitry, 3-7
 - timing diagram, 2-40
 - write procedure, 2-39 to 2-40
 - Module ID Register
 - description of, 4-2
 - digital control circuitry, 3-8
 - read procedure, 2-40
 - timing diagram, 2-40
- SCXI-1180 feedthrough panel
 - cable assembly, E-6
 - front panel installation, E-8
 - installation, E-6 to E-8
 - rear connections, E-7
- SCXI-1302 50-pin terminal block
 - cover removal, E-9
 - installation, E-9
 - wiring procedure, E-8
- SCXI-1320 terminal block, 2-21, 2-26 to 2-29, 2-32
 - installation, 2-32
- jumper configuration, 2-27
 - parts locator diagram, 2-29
 - signal connection, 2-28
 - specifications, A-3
 - temperature sensor, 2-26
 - warning on hazardous voltages, 2-21
- SCXI-1321 offset-null and shunt-calibration terminal block, 2-21 to 2-28, 2-31 to 2-32
 - installation, 2-32
 - jumper configuration, 2-27 to 2-28
 - nulling circuitry, 2-21 to 2-23
 - parts locator diagram, 2-31
 - shunt calibration, 2-24 to 2-25
 - signal connection, 2-28
 - specifications, A-3
 - temperature sensor, 2-26
 - using with RTDs and thermistors, 2-23 to 2-24
 - warning on hazardous voltages, 2-21
- SCXI-1328 high-accuracy isothermal terminal block, 2-21, 2-26 to 2-28, 2-30, 2-32
 - installation, 2-32
 - jumper configuration, 2-27
 - parts locator diagram, 2-30
 - signal connection, 2-28
 - specifications, A-3
 - temperature sensor, 2-26
 - warning on hazardous voltages, 2-21
- SCXI-1330 connector-and-shell assembly, 2-19 to 2-20
- SCXI-1340
 - cable assembly, E-1 to E-2
 - installation, E-2 to E-3
 - SCXI-1121 and MIO-16 pin equivalences, E-2
- SCXI-1341
 - cable assembly, E-3 to E-4
 - installation, E-4
 - pin translations, E-4
- SCXI-1342
 - cable assembly, E-5 to E-6
 - installation, E-6
 - pin translations, E-5
- SCXI-1343 rear screw terminal adapter
 - cable assembly, E-11
 - installation, E-11
 - pin connections, E-12
- SCXI-1344
 - cable assembly, E-3 to E-4
 - installation, E-4
 - pin translations, E-4
- SCXI-1350 multichassis adapter

- cable assembly, E-10
- installation, E-10 to E-11
- SCXI-1351 one-slot cable extender
 - cable assembly, E-9
 - installation, E-10
- SCXIbus connector, 3-2 to 3-5
 - pin assignments, 3-3, C-2
 - pin equivalences
 - with rear signal connector, 3-5
 - with SCXI-1121 and data acquisition boards, 2-36, 5-2
 - signal descriptions, 3-4 to 3-5, C-3 to C-4
- SERCLK signal
 - communicating on SPI bus, 2-37 to 2-40
 - digital I/O signal connections, 2-36
 - reading from Module ID Register, 2-40
 - rear signal connector, 2-34, B-2
 - register selection and write procedure, 5-2
 - writing the slot-select number, 2-38
 - writing to Configuration Register, 2-39
- SERDATIN signal
 - communicating on SPI bus, 2-37 to 2-40
 - digital I/O signal connections, 2-35, 2-36
 - reading from Module ID Register, 2-40
 - rear signal connector, 2-34, B-2
 - register selection and write procedure, 5-2
 - serial data timing diagram, 2-39
 - writing the slot-select number, 2-38
 - writing to Configuration Register, 2-39
- SERDATOUT signal
 - communicating on SPI bus, 2-37 to 2-40
 - digital I/O signal connections, 2-36
 - jumper connection, 2-4, 2-5 to 2-7
 - rear signal connector, 2-34, B-2
 - serial data timing diagram, 2-39
- Serial Peripheral Interface (SPI) bus
 - communications. *See* communication signals.
- shielding, grounding, and reference mode selection (jumper W33), 2-7 to 2-8
- shunt calibration circuits, 2-24 to 2-25
- signal connections
 - front connector
 - analog input channels, 2-17 to 2-19
 - excitation channels, 2-19
 - pin assignments, 2-14, D-1
 - SCXI-1320 terminal block, 2-28
 - SCXI-1321 offset-null and shunt-calibration terminal block, 2-28
 - SCXI-1328 high-accuracy isothermal terminal block, 2-28
 - SCXI-1330 connector-and-shell assembly, 2-19 to 2-20
 - signal descriptions, 2-15 to 2-17, D-2 to D-3
 - temperature sensor connection, 2-19
 - rear signal connector, 2-32 to 2-40
 - analog output signal connections, 2-35
 - communication signals, 2-37 to 2-40
 - digital I/O signal connections, 2-35 to 2-37
 - pin assignments, 2-33, B-1
 - pin equivalences with SCXIbus, 3-5
 - pin equivalences with SCXIbus and data acquisition boards, 2-36, 5-2
 - signal descriptions, 2-34 to 2-35, B-2
 - timing requirements, 2-37
 - SCXI-1320 terminal block, 2-28
 - SCXI-1321 offset-null and shunt-calibration terminal block, 2-28
 - SCXI-1328 high-accuracy isothermal terminal block, 2-28
 - SCXIbus connector, 3-2 to 3-5
 - pin assignments, 3-3, C-2
 - pin equivalences for rear signal connector, 3-5
 - pin equivalences with SCXI-1121 and data acquisition boards, 2-36
 - signal descriptions, 3-4 to 3-5, C-3 to C-4
 - warning against exceeding maximum ratings, 2-13
- single-channel measurements, 5-3 to 5-5
 - direct measurements, 5-3 to 5-4
 - multiplexed output, 5-4
 - parallel output, 5-3
 - indirect measurements, 5-4 to 5-5
 - measurements from other modules, 5-4
 - measurements from SCXI-1121 via another module, 5-5
- single-module multiplexed scanning
 - direct, 5-9
 - indirect, 5-9
- single-module parallel scanning
 - direct, 3-16 to 3-17, 5-9
 - indirect, 3-17, 5-9
- SL<3..0> bit, 4-6
- Slot 0 hardscan circuitry, programming, 5-11 to 5-12
- Slot 0 registers, 4-5 to 4-8

- FIFO Register, 4-8
- Hardscan Control Register, 4-7
- overview, 4-5
- Slot-Select Register, 4-6
- slot selection
 - slot-select timing diagram, 2-38
 - writing the slot-select number, 2-38
- SLOT0SEL* signal
 - communicating on SPI bus, 2-37 to 2-40
 - digital I/O signal connections, 2-35, 2-36
 - jumper connection, 2-4, 2-5
 - reading from Module ID Register, 2-40
 - rear signal connector, 2-34, B-2
 - register selection and write procedure, 5-2 to 5-3
 - writing the slot-select number, 2-38
 - writing to Configuration Register, 2-39
- software, optional, 1-2
- specifications
 - analog input, A-1 to A-2
 - cold-junction sensor, A-3
 - operating environment, A-4
 - physical, A-3
 - RTD mode, A-2
 - storage environment, A-4
 - strain gauge mode, A-2 to A-3
- SPI bus. *See* communication signals.
- SPICLK signal, 3-4, C-3
- SS* signal
 - communicating on SPI bus, 2-37 to 2-40
 - reading from Module ID Register, 2-40
 - SCXIBus connector, 3-5, C-4
 - writing to Configuration Register, 2-39
- storage environment specifications, A-4
- strain gauge mode specifications, A-2 to A-3

T

- technical support, G-1
- temperature sensor
 - front connector, 2-19
 - SCXI-1320 terminal block, 2-26
 - SCXI-1321 offset-null and shunt-calibration terminal block, 2-26
 - SCXI-1328 high-accuracy isothermal terminal block, 2-26
- terminal block. *See* SCXI-1302 50-pin terminal block; SCXI-1320 terminal block; SCXI-1321 offset-null and shunt-calibration terminal block; SCXI-1328 high-accuracy isothermal terminal block; SCXI-1330 connector-and-shell assembly.

- theory of operation
 - analog and timing circuitry, 3-8
 - analog input channels, 3-8 to 3-10
 - excitation output channels, 3-10
 - analog input block diagram, 3-9
 - analog output circuitry, 3-14 to 3-15
 - block diagram of SCXI-1121, 3-1
 - calibration, 3-11 to 3-13
 - equipment requirements, 3-11
 - excitation adjust, 3-12 to 3-13
 - offset null adjust, 3-12
 - potentiometers reference designators, 3-13
 - digital control circuitry, 3-7 to 3-8
 - digital interface, 3-6
 - functional overview, 3-1 to 3-5
 - scanning modes, 3-15 to 3-18
 - multiplexed scanning, 3-16 to 3-18
 - multiple-chassis scanning, 3-18
 - multiple-module multiplexed scanning, 3-17 to 3-18
 - single-module multiplexed scanning, 3-16 to 3-17
 - single-module parallel scanning, 3-15 to 3-16
 - SCXIBus connector, 3-2 to 3-5
 - pin assignments, 3-3
 - pin equivalences for rear signal connector, 3-5
 - signal descriptions, 3-4 to 3-5
 - thermistors, using with SCXI-1321, 2-23
 - timing circuitry. *See* analog and timing circuitry.
 - timing signal (SCANCLK)
 - requirements, 2-37
 - TRIG0 signal
 - analog output circuitry, 3-14
 - SCXIBus connector, 3-4, C-4

U

- unpacking the SCXI-1121, 1-4
- user-configurable jumpers, 2-4

V

- V- signal, 3-4, C-3
- V+ signal, 3-4, C-3
- Voltage excitation mode, 2-10