

PXI™-1006 Rack Mount

To mount the PXI-1006 in an instrument rack, follow the steps below.

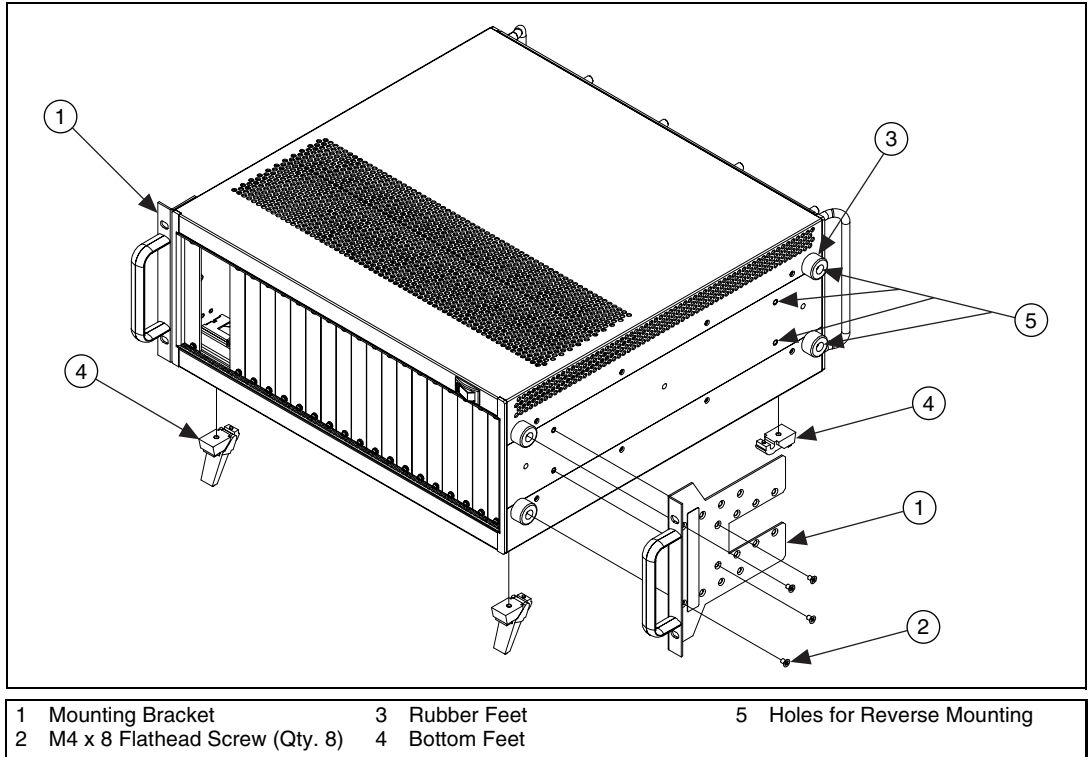


Figure 1. PXI-1006 in Rack Mount Configuration

1. Remove the rubber feet and bottom feet (as required) from the PXI-1006 chassis.
2. Install the mounting brackets onto each side of the chassis using the M4 x 8 flathead screws supplied. Note that you can recess the chassis in the cabinet rack at 1 in. increments up to 3 in. (For reverse mounting, install the brackets using the holes at the back of the chassis.)
3. Install the chassis in the instrument rack using four screws (not supplied).



323091A-01

Apr01