

CAN

NI-CAN™ Programmer Reference Manual

Worldwide Technical Support and Product Information

ni.com

National Instruments Corporate Headquarters

11500 North Mopac Expressway Austin, Texas 78759-3504 USA Tel: 512 794 0100

Worldwide Offices

Australia 03 9879 5166, Austria 0662 45 79 90 0, Belgium 02 757 00 20, Brazil 011 284 5011,
Canada (Calgary) 403 274 9391, Canada (Ontario) 905 785 0085, Canada (Québec) 514 694 8521,
China 0755 3904939, Denmark 45 76 26 00, Finland 09 725 725 11, France 01 48 14 24 24,
Germany 089 741 31 30, Greece 30 1 42 96 427, Hong Kong 2645 3186, India 91805275406,
Israel 03 6120092, Italy 02 413091, Japan 03 5472 2970, Korea 02 596 7456, Mexico (D.F.) 5 280 7625,
Mexico (Monterrey) 8 357 7695, Netherlands 0348 433466, New Zealand 09 914 0488, Norway 32 27 73 00,
Poland 0 22 528 94 06, Portugal 351 1 726 9011, Singapore 2265886, Spain 91 640 0085,
Sweden 08 587 895 00, Switzerland 056 200 51 51, Taiwan 02 2528 7227, United Kingdom 01635 523545

For further support information, see the *Technical Support Resources* appendix. To comment on the documentation, send e-mail to techpubs@ni.com

© Copyright 1996, 2000 National Instruments Corporation. All rights reserved.

Important Information

Warranty

The media on which you receive National Instruments software are warranted not to fail to execute programming instructions, due to defects in materials and workmanship, for a period of 90 days from date of shipment, as evidenced by receipts or other documentation. National Instruments will, at its option, repair or replace software media that do not execute programming instructions if National Instruments receives notice of such defects during the warranty period. National Instruments does not warrant that the operation of the software shall be uninterrupted or error free.

A Return Material Authorization (RMA) number must be obtained from the factory and clearly marked on the outside of the package before any equipment will be accepted for warranty work. National Instruments will pay the shipping costs of returning to the owner parts which are covered by warranty.

National Instruments believes that the information in this document is accurate. The document has been carefully reviewed for technical accuracy. In the event that technical or typographical errors exist, National Instruments reserves the right to make changes to subsequent editions of this document without prior notice to holders of this edition. The reader should consult National Instruments if errors are suspected. In no event shall National Instruments be liable for any damages arising out of or related to this document or the information contained in it.

EXCEPT AS SPECIFIED HEREIN, NATIONAL INSTRUMENTS MAKES NO WARRANTIES, EXPRESS OR IMPLIED, AND SPECIFICALLY DISCLAIMS ANY WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. CUSTOMER'S RIGHT TO RECOVER DAMAGES CAUSED BY FAULT OR NEGLIGENCE ON THE PART OF NATIONAL INSTRUMENTS SHALL BE LIMITED TO THE AMOUNT THEREOF PAID BY THE CUSTOMER. NATIONAL INSTRUMENTS WILL NOT BE LIABLE FOR DAMAGES RESULTING FROM LOSS OF DATA, PROFITS, USE OF PRODUCTS, OR INCIDENTAL OR CONSEQUENTIAL DAMAGES, EVEN IF ADVISED OF THE POSSIBILITY THEREOF. This limitation of the liability of National Instruments will apply regardless of the form of action, whether in contract or tort, including negligence. Any action against National Instruments must be brought within one year after the cause of action accrues. National Instruments shall not be liable for any delay in performance due to causes beyond its reasonable control. The warranty provided herein does not cover damages, defects, malfunctions, or service failures caused by owner's failure to follow the National Instruments installation, operation, or maintenance instructions; owner's modification of the product; owner's abuse, misuse, or negligent acts; and power failure or surges, fire, flood, accident, actions of third parties, or other events outside reasonable control.

Copyright

Under the copyright laws, this publication may not be reproduced or transmitted in any form, electronic or mechanical, including photocopying, recording, storing in an information retrieval system, or translating, in whole or in part, without the prior written consent of National Instruments Corporation.

Trademarks

BridgeVIEW™, CVI™, LabVIEW™, National Instruments™, NI-CAN™, ni.com™, and RTSI™ are trademarks of National Instruments Corporation.

Product and company names mentioned herein are trademarks or trade names of their respective companies.

Patents

The product described in this manual may be protected by one or more U.S. patents: U.S. Patent No. 5,938,754.

WARNING REGARDING MEDICAL AND CLINICAL USE OF NATIONAL INSTRUMENTS PRODUCTS

National Instruments products are not designed with components and testing for a level of reliability suitable for use in or in connection with surgical implants or as critical components in any life support systems whose failure to perform can reasonably be expected to cause significant injury to a human. Applications of National Instruments products involving medical or clinical treatment can create a potential for death or bodily injury caused by product failure, or by errors on the part of the user or application designer. Because each end-user system is customized and differs from National Instruments testing platforms and because a user or application designer may use National Instruments products in combination with other products in a manner not evaluated or contemplated by National Instruments, the user or application designer is ultimately responsible for verifying and validating the suitability of National Instruments products whenever National Instruments products are incorporated in a system or application, including, without limitation, the appropriate design, process and safety level of such system or application.

Compliance

FCC/Canada Radio Frequency Interference Compliance*

Determining FCC Class


The Federal Communications Commission (FCC) has rules to protect wireless communications from interference. The FCC places digital electronics into two classes. These classes are known as Class A (for use in industrial-commercial locations only) or Class B (for use in residential or commercial locations). Depending on where it is operated, this product could be subject to restrictions in the FCC rules. (In Canada, the Department of Communications (DOC), of Industry Canada, regulates wireless interference in much the same way.)

Digital electronics emit weak signals during normal operation that can affect radio, television, or other wireless products. By examining the product you purchased, you can determine the FCC Class and therefore which of the two FCC/DOC Warnings apply in the following sections. (Some products may not be labelled at all for FCC, if so the reader should then assume these are Class A devices.)

FCC Class A products only display a simple warning statement of one paragraph in length regarding interference and undesired operation. Most of our products are FCC Class A. The FCC rules have restrictions regarding the locations where FCC Class A products can be operated.

FCC Class B products display either a FCC ID code, starting with the letters **EXN**, or the FCC Class B compliance mark that appears as shown here on the right.

The curious reader can consult the FCC web site <http://www.fcc.gov> for more information.



FCC/DOC Warnings

This equipment generates and uses radio frequency energy and, if not installed and used in strict accordance with the instructions in this manual and the CE Mark Declaration of Conformity**, may cause interference to radio and television reception. Classification requirements are the same for the Federal Communications Commission (FCC) and the Canadian Department of Communications (DOC).

Changes or modifications not expressly approved by National Instruments could void the user's authority to operate the equipment under the FCC Rules.

Class A

Federal Communications Commission

This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense.

Canadian Department of Communications

This Class A digital apparatus meets all requirements of the Canadian Interference-Causing Equipment Regulations.

Cet appareil numérique de la classe A respecte toutes les exigences du Règlement sur le matériel brouilleur du Canada.

Class B

Federal Communications Commission

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful

interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

Canadian Department of Communications

This Class B digital apparatus meets all requirements of the Canadian Interference-Causing Equipment Regulations.

Cet appareil numérique de la classe B respecte toutes les exigences du Règlement sur le matériel brouilleur du Canada.

European Union - Compliance to EEC Directives

Readers in the EU/EEC/EEA must refer to the Manufacturer's Declaration of Conformity (DoC) for information** pertaining to the CE Mark compliance scheme. The Manufacturer includes a DoC for most every hardware product except for those bought for OEMs, if also available from an original manufacturer that also markets in the EU, or where compliance is not required as for electrically benign apparatus or cables.

* Certain exemptions may apply in the USA, see FCC Rules §15.103 **Exempted devices**, and §15.105(c). Also available in sections of CFR 47.

** The CE Mark Declaration of Conformity will contain important supplementary information and instructions for the user or installer.

Contents

About This Manual

How to Use the Manual Set	xi
Conventions Used in This Manual.....	xi
Related Documentation.....	xii

Chapter 1

NI-CAN Host Data Types

Chapter 2

NI-CAN Functions

ncAction	2-3
ncCloseObject	2-6
ncConfig.....	2-7
ncCreateNotification	2-12
ncCreateOccurrence	2-17
ncGetAttribute	2-20
ncOpenObject	2-22
ncRead	2-25
ncReadMult.....	2-30
ncReset.....	2-33
ncSetAttribute	2-34
ncWaitForState	2-36
ncWrite.....	2-38

Chapter 3

NI-CAN Objects

CAN Network Interface Object	3-2
CAN Object	3-17

Chapter 4

RTSI Programming

Description.....	4-1
Attributes	4-2
NC_ATTR_RTSI_MODE (RTSI Mode)	4-2
NC_RTSI_NONE (Disable RTSI)	4-2
NC_RTSI_TX_ON_IN (On RTSI Input—Transmit CAN Frame).....	4-2

NC_RTSTI_TIME_ON_IN (On RTSTI Input—Timestamp RTSTI event).....	4-3
NC_RTSTI_OUT_ON_RX (RTSTI Output on Receiving CAN frame)	4-3
NC_RTSTI_OUT_ON_TX (RTSTI Output on Transmitting CAN frame)	4-4
NC_RTSTI_OUT_ACTION_ONLY (RTSTI Output on ncAction call)	4-4
NC_ATTR_RTSTI_SIGNAL (RTSTI Line Number).....	4-4
NC_ATTR_RTSTI_SIG_BEHAV (RTSTI Behavior).....	4-4
NC_ATTR_RTSTI_FRAME (UserRTSTIFrame)	4-5
NC_ATTR_RTSTI_SKIP (RTSTI Skip).....	4-5
Examples	4-5

Appendix A NI-CAN Object States

Appendix B Status Codes and Qualifiers

Appendix C Technical Support Resources

Glossary

Index

Figures

Figure 3-1. Example of Periodic Transmission	3-32
Figure 3-2. Example of Polling Remote Data Using ncWrite	3-32
Figure 3-3. Example of Periodic Polling of Remote Data.....	3-33
Figure A-1. State Format	A-1
Figure B-1. Status Format	B-1

Tables

Table 1-1. NI-CAN Host Data Types	1-1
Table 2-1. NI-CAN Functions.....	2-2
Table 2-2. Actions Supported by the CAN Network Interface Object	2-4
Table 2-3. Actions Supported by the CAN Object.....	2-5
Table 2-4. NCTYPE_CAN_FRAME_TIMED Field Names	2-27
Table 2-5. NCTYPE_CAN_DATA_TIMED Field Names	2-29

Table 2-6.	NCTYPE_CAN_FRAME Field Names	2-39
Table 2-7.	NCTYPE_CAN_DATA Field Name	2-40
Table A-1.	NI-CAN Object States	A-1
Table B-1.	Determining Severity of Status	B-2
Table B-2.	Summary of Status Codes	B-4

About This Manual

This manual is a programming reference for functions, objects, and data types in the NI-CAN software. This manual assumes that you are already familiar with the Windows system you are using.

How to Use the Manual Set

Use the getting started manual to install and configure your CAN hardware and NI-CAN software.

Use the *NI-CAN User Manual* to learn the basics of NI-CAN and how to develop an application. The user manual also contains debugging information and examples.

Use this *NI-CAN Programmer Reference Manual* for specific information about each NI-CAN function and object, such as format, parameters, and possible errors.

Conventions Used in This Manual



The following conventions appear in this manual:

This icon denotes a note, which alerts you to important information.

bold

Bold text denotes items that you must select or click on in the software, such as menu items and dialog box options. Bold text also denotes parameter names.

italic

Italic text denotes variables, emphasis, a cross reference, or an introduction to a key concept. This font also denotes text that is a placeholder for a word or value that you must supply.

`monospace`

Text in this font denotes text or characters that you should enter from the keyboard, sections of code, programming examples, and syntax examples. This font is also used for the proper names of disk drives, paths, directories, programs, subprograms, subroutines, device names, functions, operations, variables, filenames and extensions, and code excerpts.

monospace italic

Italic text in this font denotes text that is a placeholder for a word or value that you must supply.

Related Documentation

The following documents contain information that you might find helpful as you read this manual:

- *ANSI/ISO Standard 11898-1993, Road Vehicles—Interchange of Digital Information—Controller Area Network (CAN) for High-Speed Communication*
- *ANSI/ISO Standard 11519-1, 2 Road Vehicles—Low Speed Serial Data Communications, Part 1 and 2*
- *CAN Specification Version 2.0*, 1991, Robert Bosch GmbH., Postfach 500, D-7000 Stuttgart 1
- LabVIEW Online Reference
- Win32 Software Development Kit (SDK) online help

NI-CAN Host Data Types

This chapter describes the host data types used by NI-CAN functions and objects.

All host data types are given specific names for reference within this manual. In general, all NI-CAN host data types begin with `NCTYPE_`.

Table 1-1. NI-CAN Host Data Types

NI-CAN Data Type	ANSI C Binding	LabVIEW Binding	Description
<code>NCTYPE_type_P</code>	<code>NCTYPE_type *</code>	N/A	Location of variable with type <i>type</i> .
<code>NCTYPE_INT8</code>	signed char	I8	8-bit signed integer.
<code>NCTYPE_INT16</code>	signed short	I16	16-bit signed integer.
<code>NCTYPE_INT32</code>	signed long	I32	32-bit signed integer.
<code>NCTYPE_UINT8</code>	unsigned char	U8	8-bit unsigned integer.
<code>NCTYPE_UINT16</code>	unsigned short	U16	16-bit unsigned integer.
<code>NCTYPE_UINT32</code>	unsigned long	U32	32-bit unsigned integer.
<code>NCTYPE_BOOL</code>	<code>NCTYPE_UINT8</code>	TF (boolean)	Boolean value. In ANSI C, constants <code>NC_TRUE</code> (1) and <code>NC_FALSE</code> (0) are used for comparisons.
<code>NCTYPE_STRING</code>	<code>char *</code> , array of characters terminated by null character <code>\0</code>	abc (string)	ASCII character string.
<code>NCTYPE_ANY_P</code>	<code>void *</code>	N/A	Reference to variable of unknown type, used in cases where actual data type may vary depending on particular context.

Table 1-1. NI-CAN Host Data Types (Continued)

NI-CAN Data Type	ANSI C Binding	LabVIEW Binding	Description
NCTYPE_OBJH	NCTYPE_UINT32	Type definition ObjHandle (U32)	Handle referring to object.
NCTYPE_VERSION	NCTYPE_UINT32	U32	Version number. Major, minor, subminor, and beta version numbers are encoded in unsigned 32-bit integer from high byte to low byte. Letters are encoded as numeric equivalents ('A' is 1, 'Z' is 26, and so on.). Version 2.0B would be hexadecimal 02000200, and Beta version 1.4.2 beta 7 would be hex 01040207.
NCTYPE_DURATION	NCTYPE_UINT32	U32	Time duration indicating elapsed time between two events. Time is expressed in 1 ms increments. 10 seconds is 10000. Special constant NC_DURATION_NONE (0) is used for zero duration, and NC_DURATION_INFINITE (FFFFFFFF hex) is used for infinite duration.
NCTYPE_ABS_TIME	unsigned 64-bit integer compatible with the Win32 FILETIME type	64-bit double-precision floating-point (DBL) compatible with LabVIEW time	For information on use, refer to ncRead function description in Chapter 2, NI-CAN Functions .
NCTYPE_ATTRID	NCTYPE_UINT32	U32	Attribute identifier.
NCTYPE_OPCODE	NCTYPE_UINT32	U32	Operation code used with ncAction function.

Table 1-1. NI-CAN Host Data Types (Continued)

NI-CAN Data Type	ANSI C Binding	LabVIEW Binding	Description
NCTYPE_PROTOCOL	NCTYPE_UINT32	U32	Supported device network protocol, such as NC_PROTOCOL_CAN (1).
NCTYPE_BAUD_RATE	NCTYPE_UINT32	U32	Baud rate. 125 kb/s would be encoded as 125000.
NCTYPE_STATE	NCTYPE_UINT32	U32	Object states, encoded as 32-bit mask (one bit for each state). For information, refer to Appendix A, <i>NI-CAN Object States</i> .
NCTYPE_STATUS	NCTYPE_INT32	I32	Status returned from all NI-CAN functions. Status is zero for success, less than zero for an error, and greater than zero for a warning. For information, refer to Appendix B, <i>Status Codes and Qualifiers</i> .
NCTYPE_CAN_ARBID	NCTYPE_UINT32	U32	CAN arbitration ID. 30th bit is accessed using bitmask NC_FL_CAN_ARBID_XTD (20000000 hex). If this bit is clear, CAN arbitration ID is standard (11-bit). If this bit is set, CAN arbitration ID is extended (29-bit). Special constant NC_CAN_ARBID_NONE (CFFFFFFF hex) indicates no CAN arbitration ID.

Table 1-1. NI-CAN Host Data Types (Continued)

NI-CAN Data Type	ANSI C Binding	LabVIEW Binding	Description
NCTYPE_CAN_FRAME	struct	Input terminals of ncWriteNet.vi	Structure used with ncWrite and CAN Network Interface Object. For information, refer to description of CAN Network Interface Object in Chapter 3, <i>NI-CAN Objects</i> .
NCTYPE_CAN_FRAME_TIMED	struct	Output terminals of ncReadNet.vi and ncReadMult.vi	Structure used with ncRead and CAN Network Interface Object. For information, refer to description of CAN Network Interface Object in Chapter 3, <i>NI-CAN Objects</i> .
NCTYPE_CAN_DATA	struct	Input terminals of ncWriteObj.vi	Structure used with ncWrite and CAN Object. For information, refer to description of CAN Object in Chapter 3, <i>NI-CAN Objects</i> .
NCTYPE_CAN_DATA_TIMED	struct	Output terminals of ncReadObj.vi and ncReadObjMult.vi	Structure used with ncRead and CAN Object For information, refer to description of CAN Object in Chapter 3, <i>NI-CAN Objects</i> .

NI-CAN Functions

This chapter lists the NI-CAN functions and describes the format, purpose, parameters, and return status for each function.

Unless otherwise stated, each NI-CAN function suspends execution of the calling process until it completes.

Function Names

The functions in this chapter are listed alphabetically.

Purpose

Each function description includes a brief statement of the purpose of the function.

Format

The format section describes the format of each function for LabVIEW, and for the C programming language.

Input and Output

The input and output parameters for each function are listed.

Description

The description section gives details about the purpose and effect of each function.

CAN Network Interface Object

The CAN Network Interface Object section gives details about using the function with the CAN Network Interface Object.

CAN Object

The CAN Object section gives details about using the function with the CAN Object.

Return Status

After every NI-CAN function description, all possible return status codes are listed. For complete information on status format and the qualifiers used with each status code, refer to Appendix B, *Status Codes and Qualifiers*.

Examples

Each function description includes sample C language code showing how to use the function. For more detailed examples or for example LabVIEW code, refer to the example programs that are included with your NI-CAN software. The example programs are described in the *NI-CAN User Manual*.

List of NI-CAN Functions

The following table contains an alphabetical list of the NI-CAN functions.

Table 2-1. NI-CAN Functions

Function	Purpose
ncAction	Perform an action on an object.
ncCloseObject	Close an object.
ncConfig	Configure an object prior to its use.
ncCreateNotification	Create a notification callback for an object (C only).
ncCreateOccurrence	Create a notification occurrence for an object (LabVIEW only).
ncGetAttribute	Get the value of an object's attribute.
ncOpenObject	Open an object.
ncRead	Read the data value of an object.
ncReadMult	Read multiple data values from an object.
ncReset	Reset CAN interface.
ncSetAttribute	Set the value of an object's attribute.
ncWaitForState	Wait for one or more states to occur in an object.
ncWrite	Write the data value of an object.


ncAction

Purpose

Perform an action on an object.

Format

LabVIEW



C

```
NCTYPE_STATUS ncAction(NCTYPE_OBJH ObjHandle,
NCTYPE_OPCODE Opcode,
NCTYPE_UINT32 Param)
```

Input

ObjHandle	Object handle.
Opcode	Operation code indicating which action to perform.
Param	Parameter whose meaning is defined by Opcode.

Description

`ncAction` is a general purpose function you can use to perform an action on the object specified by `ObjHandle`. Its normal use is to start and stop network communication on a CAN Network Interface Object.

For the most frequently used and/or complex actions, NI-CAN provides functions such as `ncOpenObject` and `ncRead`. `ncAction` provides an easy, general purpose way to perform actions that are used less frequently or are relatively simple.

CAN Network Interface Object

NI-CAN propagates all actions on the CAN Network Interface Object up to all open CAN Objects. Table 2-2 describes the actions supported by the CAN Network Interface Object.

Table 2-2. Actions Supported by the CAN Network Interface Object

Opcode	Param	Description
NC_OP_START (80000001 hex)	N/A (ignored)	Transitions network interface from stopped (idle) state to started (running) state. If network interface is already started, this operation has no effect. When a network interface is started, it is communicating on the network. When you execute NC_OP_START on a stopped CAN Network Interface Object, NI-CAN propagates it upward to all open higher-level CAN Objects. Thus, you can use it to start all higher-level network communication simultaneously.
NC_OP_STOP (80000002 hex)	N/A (ignored)	Transitions network interface from started state to stopped state. If network interface is already stopped, this operation has no effect. When a network interface is stopped, it is not communicating on the network. When you execute NC_OP_STOP on a running CAN Network Interface Object, NI-CAN propagates it upward to all open higher-level CAN Objects.
NC_OP_RESET (80000003 hex)	N/A (ignored)	Resets network interface. Stops network interface, then resets the CAN chip to clear the CAN error counters (clear error passive state). Resetting includes clearing all entries from read and write queues. NC_OP_RESET is propagated up to all open higher-level CAN Objects.
NC_OP_RTISI_OUT (80000004 hex)	N/A (ignored)	Output a pulse or toggle on the RTSI line depending upon the NC.ATTR.RTISI.SIG.BEHAV

CAN Object

All actions performed on a CAN Object affect that CAN Object alone, and do not affect other CAN Objects or communication as a whole. To start communications for a CAN Object, you must first start its lower-level CAN Network Interface Object. After starting communications, you can then use `ncAction` to stop and restart an individual CAN Object.

Table 2-3 describes the actions supported by the CAN Object.

Table 2-3. Actions Supported by the CAN Object

Opcode	Param	Description
NC_OP_START (80000001 hex)	N/A (ignored)	When NC_OP_STOP is used to stop a CAN Object, NC_OP_START restarts the CAN Object. This action does not start the CAN Object unless the lower-level CAN Network Interface Object is started (running).
NC_OP_STOP (80000002 hex)	N/A (ignored)	Stops the CAN Object. For example, if the CAN Object is configured to transmit data frames periodically, this action stops the periodic transmissions.
NC_OP_RESET (80000003 hex)	N/A (ignored)	Resets the CAN Object. Stops the CAN Object, then clears all entries from read and write queues.
NC_OP_RTSM_OUT (80000004 hex)	N/A (ignored)	Output a pulse or toggle on the RTSI line depending upon the NC.ATTR.RTSM.SIG.BEHAV

Return Status

NC_SUCCESS	Success (no warning or error).
NC_ERR_BAD_PARAM	Invalid parameter.
NC_ERR_BAD_VALUE	Invalid values for configuration attributes. Returned only when Opcode is NC_OP_START.
NC_ERR_DRIVER	Implementation-specific error in the NI-CAN driver.

Example

This example assumes the following declarations:

```
NCTYPE_STATUS      status;
NCTYPE_OBJH        objh;
```

Start communication on a CAN Network Interface Object. Because Param is ignored for NC_OP_START, you can use any value (this example uses 0).

```
status = ncAction(objh, NC_OP_START, 0);
```


ncCloseObject

Purpose

Close an object.

Format

LabVIEW



C

```
NCTYPE_STATUS    ncCloseObject (NCTYPE_OBJH ObjHandle)
```

Input

ObjHandle Object handle.

Description

ncCloseObject closes an object when it no longer needs to be in use, such as when the application is about to exit. When an object is closed, NI-CAN stops all pending operations and clears RTSI configuration for the object, and you can no longer use the ObjHandle in your application.

CAN Network Interface Object

ObjHandle refers to an open CAN Network Interface Object.

CAN Object

ObjHandle refers to an open CAN Object.

Return Status

NC_SUCCESS	Success (no warning or error).
NC_ERR_BAD_PARAM	Invalid parameter.
NC_ERR_DRIVER	Implementation-specific error in the NI-CAN driver.

Example

This example assumes the following declarations:

```
NCTYPE_STATUS    status;
NCTYPE_OBJH     objh;
```

Close an object.

```
status = ncCloseObject (objh);
```


ncConfig

Purpose

Configure an object before using it.

Format

LabVIEW

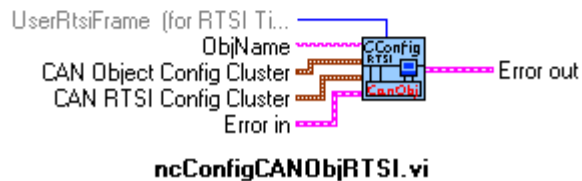

C

NCTYPE_STATUS

```
ncConfig(NCTYPE_STRING ObjName,
NCTYPE_UINT32 NumAttrs,
NCTYPE_ATTRID_P AttrIdList,
NCTYPE_UINT32_P AttrValueList)
```

Input

<code>ObjName</code>	ASCII name of the object to configure.
<code>NumAttrs</code>	Number of configuration attributes (C only).
<code>AttrIdList</code>	List of configuration attribute identifiers (C only).
<code>AttrValueList</code>	List of configuration attribute values (C only).
<code>ConfigCluster</code>	Cluster of object-specific configuration attribute values (LabVIEW only).
<code>RTSIConfigCluster</code>	Cluster of object-specific RTSI configuration attribute values (LabVIEW only). This is an optimal input.

Description

`ncConfig` initializes the configuration attributes of an object before opening it. If you have configured objects using the NI-CAN Configuration utility, you might not need to call this function in your application. For any object, `ncConfig` overrides the configuration specified in the NI-CAN Configuration utility, if any. `ncConfig` also initiates a cable-detect test and reports any configuration errors for the new PCMCIA-CAN cards that support all types of National Instruments PCMCIA-CAN cables. For example, you can attach a high-speed cable and communicate with high-speed devices at rates up to 1MB/sec. Using the same PCMCIA card you can attach a low-speed cable, fault tolerant up to 125Kbits/sec, and communicate with low-speed devices.

`ObjName` uses the same object hierarchy syntax as `ncOpenObject`; it cannot be a user-defined alias.

`NumAttr` indicates the number of configuration attributes in `AttrIdList` and `AttrValueList`. `AttrIdList` is an array of attribute IDs, and `AttrValueList` is an array of values. The attributes in `AttrIdList` must have `Config` permissions in the description of the object. The host data type for each value in `AttrValueList` is `NCTYPE_UINT32`, which all configuration attributes can use.

Attributes with `Config` permissions must be initialized prior to opening the object, and cannot be changed using `ncSetAttribute`.

Using the LabVIEW Configuration Functions

The LabVIEW configuration functions do not require the input parameters `AttrIdList` and `NumAttrs`. The configuration attribute values are instead provided in an object-specific cluster. Controls for these configuration clusters can be found in the NI-CAN Controls palette, one for the CAN Network Interface Object (`ncNetAttr.ctl`), one for the CAN Object (`ncObjAttr.ctl`), one for RTSI (`ncCANRtsiAttr.ctl`) and one for DAQ/CAN synchronization configuration (`CAN/DAQConfig.ctl`). Note that the attribute names in the RTSI configuration cluster are made descriptive for easy understandability.

The `ConfigCluster` input can be programmed in one of the following ways:

- Place the appropriate control on your front panel, then wire that control into the `ConfigCluster` input.
- Right-click on the `ConfigCluster` input and select **Create Control**. This control will not maintain the format, defaults, or description of the original.
- Right-click on the `ConfigCluster` input and select **Create Constant**. This constant will not maintain the format, defaults, or description of the original.

CAN Network Interface Object

The following are the `Config` attributes of the CAN Network Interface Object:

`NC_ATTR_BAUD_RATE` (Baud Rate)
`NC_ATTR_START_ON_OPEN` (Start on Open)
`NC_ATTR_READ_Q_LEN` (Read Queue Length)
`NC_ATTR_WRITE_Q_LEN` (Write Queue Length)
`NC_ATTR_CAN_COMP_STD` (Standard Comparator)
`NC_ATTR_CAN_MASK_STD` (Standard Mask)
`NC_ATTR_CAN_COMP_XTD` (Extended Comparator)
`NC_ATTR_CAN_MASK_XTD` (Extended Mask)
`NC_ATTR_LOG_COMM_ERRS` (Low-speed CAN only)
`NC_ATTR_RTSMODE` (RTSM Mode)
`NC_ATTR_RTSM_SIGNAL` (RTSM Line Selector)
`NC_ATTR_RTSM_SIG_BEHAV` (RTSM Signal Behavior)
`NC_ATTR_RTSM_SKIP` (Number of RTSM Triggers to Skip)
`NC_ATTR_READ_MULT_SIZE` (Size to Be Used with Notifications or Occurrences)

For more information on these configuration attributes, as well as usage of `ObjName`, refer to the [CAN Network Interface Object](#) section of Chapter 3, *NI-CAN Objects*.

CAN Object

The following are the `Config` attributes of the CAN Object:

`NC_ATTR_PERIOD` (Period)
`NC_ATTR_READ_Q_LEN` (Read Queue Length)
`NC_ATTR_WRITE_Q_LEN` (Write Queue Length)
`NC_ATTR_RX_CHANGES_ONLY` (Receive Changes Only)
`NC_ATTR_COMM_TYPE` (Communication Type)
`NC_ATTR_CAN_TX_RESPONSE` (Transmit by Response)
`NC_ATTR_CAN_DATA_LENGTH` (Data Length)
`NC_ATTR_RTSMODE` (RTSM Mode)
`NC_ATTR_RTSM_SIGNAL` (RTSM Line Selector)
`NC_ATTR_RTSM_SIG_BEHAV` (RTSM Signal Behavior)
`NC_ATTR_RTSM_SKIP` (Number of RTSM Triggers to Skip)

NC_ATTR_READ_MULT_SIZE (Size to Be Used with Notifications or Occurances)
 NC_ATTR_RTSTI_FRAME (User-Defined Data Frame)

For more information on these configuration attributes, as well as usage of ObjName, refer to the *CAN Network Interface Object* section of Chapter 3, *NI-CAN Objects*.

Return Status

NC_SUCCESS	Success (no warning or error).
NC_ERR_BAD_NAME	Invalid or unrecognized name in ObjName.
NC_ERR_BAD_PARAM	Invalid parameter.
NC_ERR_ALREADY_OPEN	Object already opened.
NC_ERR_DRIVER	Implementation-specific error in the NI-CAN driver.
NC_ERR_BAD_VALUE	Invalid values for configuration attributes.

Example

This example assumes the following declarations:

```
NCTYPE_STATUS      status;
NCTYPE_OBJH        objh;
NCTYPE_ATTRID      AttrIdList [8];
NCTYPE_UINT32      AttrValueList [8];
```

Configure a CAN Network Interface Object.

```
AttrIdList [0] = NC_ATTR_BAUD_RATE;
AttrValueList [0] = 125000;
AttrIdList [1] = NC_ATTR_START_ON_OPEN;
AttrValueList [1] = NC_TRUE;
AttrIdList [2] = NC_ATTR_READ_Q_LEN;
AttrValueList [2] = 10;
AttrIdList [3] = NC_ATTR_WRITE_Q_LEN;
AttrValueList [3] = 10;
AttrIdList [4] = NC_ATTR_CAN_COMP_STD;
AttrValueList [4] = 0;
AttrIdList [5] = NC_ATTR_CAN_MASK_STD;
AttrValueList [5] = 0;
AttrIdList [6] = NC_ATTR_CAN_COMP_XTD;
AttrValueList [6] = 0;
AttrIdList [7] = NC_ATTR_CAN_MASK_XTD;
AttrValueList [7] = 0;
status = ncConfig ("CAN0", 8, AttrIdList, AttrValueList);
```

Configure a CAN Interface Object for low-speed CAN.

All of the above `AttrIdList` and `AttrValueList` (as needed) as well as the following:

```
AttrIdList[8] = NC_ATTR_LOG_COMM_ERRS;
AttrValueList[8] = NC_TRUE;
```

Configure RTSI for Network Interface Object.

All of the above `AttrIdList` and `AttrValueList` (as needed) as well as the following:

```
AttrIdList[8] = NC_ATTR_RTSI_MODE;
AttrValueList[8] = NC_RTSI_OUT_ON_TX;
AttrIdList[9] = NC_ATTR_RTSI_SIGNAL;
AttrValueList[9] = 4;
AttrIdList[10] = NC_ATTR_RTSI_SIG_BEHAV;
AttrValueList[10] = NC_RTSI_SIG_PULSE;
AttrIdList[11] = NC_ATTR_RTSI_SKIP;
```

Configure RTSI for CAN Object.

```
AttrIdList[7] = NC_ATTR_RTSI_MODE;
AttrValueList[7] = NC_RTSI_TIME_ON_IN;
AttrIdList[8] = NC_ATTR_RTSI_SIGNAL;
AttrValueList[8] = 4;
AttrIdList[9] = NC_ATTR_RTSI_FRAME;
AttrValueList[9] = 0xAABBCCDD;
AttrValueList[11] = 5;
```

ncCreateNotification

Purpose

Create a notification callback for an object (C only).

Format

LabVIEW

N/A (`ncCreateOccurrence` serves a similar purpose.)

C

```
NCTYPE_STATUS      ncCreateNotification(NCTYPE_OBJH ObjHandle,
                                         NCTYPE_STATE DesiredState,
                                         NCTYPE_DURATION Timeout,
                                         NCTYPE_ANY_P RefData,
                                         NCTYPE_NOTIFY_CALLBACK
                                         Callback)
```

Input

<code>ObjHandle</code>	Object handle.
<code>DesiredState</code>	States for which notification is sent.
<code>Timeout</code>	Length of time to wait.
<code>RefData</code>	Pointer to user-specified reference data.
<code>Callback</code>	Address of your callback function.

Description

`ncCreateNotification` creates a notification callback for the object specified by `ObjHandle`. The NI-CAN driver uses the notification callback to communicate state changes to your application. The `ncCreateNotification` function is not applicable to LabVIEW programming. Use the `ncCreateOccurrence` function to receive notifications within LabVIEW.

This function is normally used when you want to allow other code to execute while waiting for NI-CAN states, especially when the other code does not call NI-CAN functions. If such background execution is not needed, the `ncWaitForState` function offers better overall performance. The `ncWaitForState` function cannot be used at the same time as `ncCreateNotification`.

Upon successful return from `ncCreateNotification`, the notification callback is invoked whenever one of the states specified by `DesiredState` occurs in the object. If `DesiredState` is zero, notifications are disabled for the object specified by `ObjHandle`.

The NI-CAN driver waits up to `Timeout` for one of the bits set in `DesiredState` to become set in the attribute `NC_ATTR_STATE`. You can use the special `Timeout` value `NC_DURATION_INFINITE` to wait indefinitely.

The `Callback` parameter provides the address of a callback function in your application. Within the `Callback` function, you can call any of the NI-CAN functions except `ncCreateNotification` and `ncWaitForState`.

With the `RefData` parameter, you provide a pointer that is sent to all notifications for the given object. This pointer normally provides reference data for use within the `Callback` function. For example, when you create a notification for the `NC_ST_READ_AVAIL` state, `RefData` is often the data pointer that you pass to `ncRead` to read available data. If the callback function does not need reference data, you can set `RefData` to `NULL`.

Callback Prototype

```
NCTYPE_STATE      _NCFUNC_ Callback (NCTYPE_OBJH ObjHandle,
                                     NCTYPE_STATE State,
                                     NCTYPE_STATUS Status,
                                     NCTYPE_ANY_P RefData);
```

Callback Parameters

<code>ObjHandle</code>	Object handle.
<code>State</code>	Current state of object.
<code>Status</code>	Object status.
<code>RefData</code>	Pointer to your reference data.

Callback Return Value

The value you return from the callback indicates the desired states to re-enable for notification. If you no longer want to receive notifications for the callback, return a value of zero.

If you return a state from the callback, and that state is still set in the `NC_ATTR_STATE` attribute, the callback is invoked again immediately after it returns. For example, if you return `NC_ST_READ_AVAIL` when the read queue has not been emptied, the callback is invoked again.

Callback Description

In the prototype for `Callback`, `_NCFUNC_` ensures a proper calling scheme between the NI-CAN driver and your callback.

The `Callback` function executes in a separate thread in your process. Therefore, it has access to any process global data, but not to thread local data. If the callback needs to access global data, you must protect that access using synchronization primitives (such as semaphores), because the callback is running in a different thread context. Alternatively, you can avoid the issue of data protection entirely if the callback simply posts a message to your application using the Win32 `PostMessage` function. For complete information on multithreading issues, refer to the Win32 Software Development Kit (SDK) online help.

The `ObjHandle` is the same object handle passed to `ncCreateNotification`. It identifies the object generating the notification, which is useful when you use the same callback function for notifications from multiple objects.

The `State` parameter holds the current state of the object that generated the notification (`NC_ATTR_STATE` attribute). If the `Timeout` passed to `ncCreateNotification` expires before the desired states occur, the NI-CAN driver invokes the callback with `State` equal to zero.

The `Status` parameter holds the current status of the object. If the notification is sent for the background error and warning states (`NC_ST_ERROR` or `NC_ST_WARNING`), `Status` holds the background status attribute (`NC_ATTR_STATUS`) of the object. If an error occurs with the notification, `State` is zero and `Status` holds the error status. The most common notification error occurs when the `Timeout` passed to `ncCreateNotification` expires before the desired states occur (`NC_ERR_TIMEOUT` status code with `NC_QUAL_TIMO_FUNCTION` qualifier). If no background error or warning is reported, and no notification error occurred, `Status` is `NC_SUCCESS`.

The `RefData` parameter is the same pointer passed to `ncCreateNotification`, and it accesses reference data for the `Callback` function.

CAN Network Interface Object

The following states apply to the CAN Network Interface Object:

<code>NC_ST_READ_AVAIL</code>	Frame received, available for <code>ncRead</code> .
<code>NC_ST_WRITE_SUCCESS</code>	Frames written with <code>ncWrite</code> were successfully transmitted.
<code>NC_ST_STOPPED</code>	Communication stopped.
<code>NC_ST_ERROR</code>	Error occurred in background.
<code>NC_ST_WARNING</code>	Warning occurred in background.
<code>NC_ST_READ_MULT</code>	Multiple frames available in Read Queue (to be used with <code>ncReadMult</code>).

For more information on these states and the bit values used for each, refer to Appendix A, *NI-CAN Object States*.

CAN Object

The following states apply to the CAN Object:

NC_ST_READ_AVAIL	Data received, available for <code>ncRead</code> .
NC_ST_WRITE_SUCCESS	Data or remote frames written with <code>ncWrite</code> were successfully transmitted.
NC_ST_STOPPED	CAN Object behavior stopped.
NC_ST_ERROR	Error occurred in background.
NC_ST_WARNING	Warning occurred in background.
NC_ST_READ_MULT	Multiple frames available in Read Queue (to be used with <code>ncReadMult</code>).

For more information on these states and the bit values used for each, refer to Appendix A, *NI-CAN Object States*.

Return Status

NC_SUCCESS	Success (no warning or error).
NC_ERR_BAD_PARAM	Invalid parameter.
NC_ERR_DRIVER	Implementation-specific error in the NI-CAN driver.

Example

Create a notification for the `NC_ST_READ_AVAIL` state.

```
NCTYPE_STATE      _NCFUNC_ MyCallback (NCTYPE_OBJH ObjHandle,
                                         NCTYPE_STATE State,
                                         NCTYPE_STATUS Status,
                                         NCTYPE_ANY_P RefData){
    .
    .
    .
}
```

```
void main()      {
NCTYPE_STATUS    status;
NCTYPE_OBJH      objh
    .
    .
    .
/* Create notification to handle data available in read queue. The
notification waits indefinitely. No RefData is used.*/
```

```
status = ncCreateNotification (objh, NC_ST_READ_AVAIL,  
NC_DURATION_INFINITE, NULL, MyCallback);  
.   
.   
.   
}
```


ncCreateOccurrence

Purpose

Create a notification occurrence for an object (LabVIEW only).

Format

LabVIEW



C

N/A (ncCreateNotification serves a similar purpose.)

Input

ObjHandle	Object handle.
DesiredState	States for which notification is sent.

Output

Occurrence	Occurrence that can be used with LabVIEW Wait on Occurrence VI .
------------	-------------------------------------------------------------------------

Description

ncCreateOccurrence creates a notification occurrence for the object specified by ObjHandle. The NI-CAN driver uses the occurrence callback to communicate state changes to your application. The ncCreateOccurrence function is not applicable to C programming. Use the ncCreateNotification function to receive notifications within C.

This function is normally used when you want to allow other code to execute while waiting for NI-CAN states, especially when the other code does not call NI-CAN functions. If such background execution is not needed, the ncWaitForState function offers better overall performance. The ncWaitForState function cannot be used at the same time as ncCreateOccurrence.

Upon successful return from ncCreateOccurrence, the notification occurrence is invoked whenever one of the states specified by DesiredState occurs in the object. If DesiredState is zero, notifications are disabled for the object specified by ObjHandle.

The Occurrence output is normally wired into the LabVIEW **Wait on Occurrence VI**. **Wait on Occurrence** takes the Occurrence, and also a timeout and flag indicating whether

to ignore a pending state. For more information on **Wait On Occurrence**, refer to the LabVIEW Online Reference.

When **Wait on Occurrence** completes, you should execute code to handle the `DesiredState`. For example:

1. if `DesiredState` is `NC_ST_READ_AVAIL`, you should call `ncRead` to read the available data.
2. if `DesiredState` is `NC_ST_READ_MULT`, you should call `ncReadMult` to read the available data.

After it has been created, the `Occurrence` will be set each time a `DesiredState` goes from false to true. When you no longer want to wait on the `Occurrence` (for example, when terminating your application), call `ncCreateOccurrence` with `DesiredState` zero.

CAN Network Interface Object

The following states apply to the CAN Network Interface Object:

<code>NC_ST_READ_AVAIL</code>	Frame received, available for <code>ncRead</code> .
<code>NC_ST_WRITE_SUCCESS</code>	Frames written with <code>ncWrite</code> were successfully transmitted.
<code>NC_ST_STOPPED</code>	Communication stopped.
<code>NC_ST_ERROR</code>	Error occurred in background.
<code>NC_ST_WARNING</code>	Warning occurred in background.
<code>NC_ST_READ_MULT</code>	Multiple frames available in Read Queue for <code>ncReadMult</code> .

For more information on these states and the bit values used for each, refer to Appendix A, [NI-CAN Object States](#).

CAN Object

The following states apply to the CAN Object:

<code>NC_ST_READ_AVAIL</code>	Data received, available for <code>ncRead</code> .
<code>NC_ST_WRITE_SUCCESS</code>	Data or remote frames written with <code>ncWrite</code> were successfully transmitted.
<code>NC_ST_STOPPED</code>	CAN Object behavior stopped.
<code>NC_ST_ERROR</code>	Error occurred in background.
<code>NC_ST_WARNING</code>	Warning occurred in background.
<code>NC_ST_READ_MULT</code>	Multiple frames available in Read Queue for <code>ncReadMult</code> .


For more information on these states and the bit values used for each, refer to Appendix A, [NI-CAN Object States](#).

Return Status

<code>NC_SUCCESS</code>	Success (no warning or error).
<code>NC_ERR_BAD_PARAM</code>	Invalid parameter.
<code>NC_ERR_DRIVER</code>	Implementation-specific error in the NI-CAN driver.

Example

Create an occurrence that sets when data is available to be read. Inside a loop, read a CAN frame whenever the occurrence sets. If the occurrence times out after 10 seconds, break from the loop.

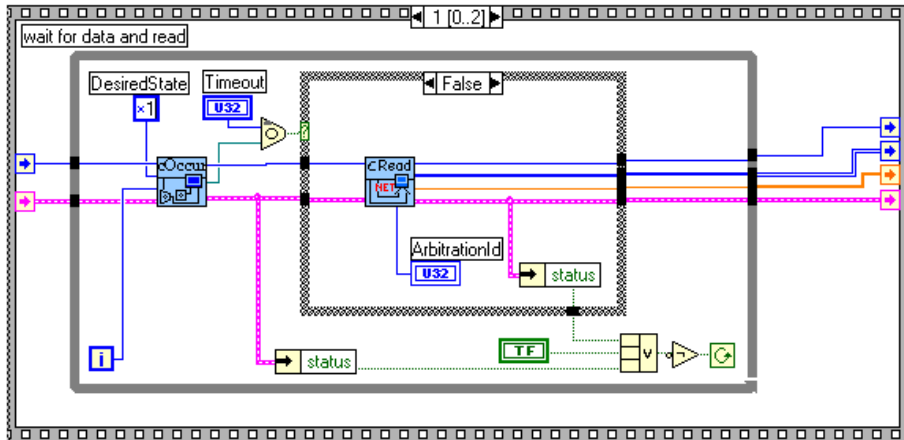

ncGetAttribute

Purpose

Get the value of an object attribute.

Format

LabVIEW



C

```
NCTYPE_STATUS      ncGetAttribute(NCTYPE_OBJH ObjHandle,
                                NCTYPE_ATTRID AttrId,
                                NCTYPE_UINT32 AttrSize,
                                NCTYPE_ANY_P AttrPtr)
```

Input

ObjHandle	Object handle.
AttrId	Identifier of the attribute to get.
AttrSize	Size of the attribute in bytes (C only).

Output

AttrPtr (AttrValue)	Returned attribute value. For C, the attribute value is returned to you using the pointer AttrPtr. For LabVIEW, the attribute value is returned to you in AttrValue.
---------------------	----------------------------------------------------------------------------------------------------------------------------------------------------------------------

Description

ncGetAttribute gets the value of the attribute specified by AttrId from the object specified by ObjHandle. Within NI-CAN objects, you use attributes to access configuration settings, status, and other information about the object, but not data.

For C, AttrPtr points to the variable used to receive the attribute value. Its type is undefined so that you can use the appropriate host data type for AttrId. AttrSize indicates the size of the variable that AttrPtr points to.

For LabVIEW, this function gets the value of an object's attribute into a LabVIEW U32 (AttrValue), so a size is not needed.

CAN Network Interface Object

For information on the attributes of the CAN Network Interface Object, refer to the [CAN Network Interface Object](#) section of Chapter 3, *NI-CAN Objects*.

CAN Object

For information on the attributes of the CAN Object, refer to the [CAN Object](#) section of Chapter 3, *NI-CAN Objects*.

Return Status

NC_SUCCESS	Success (no warning or error).
NC_ERR_BAD_PARAM	Invalid parameter.
NC_ERR_DRIVER	Implementation-specific error in the NI-CAN driver.

Example

This example assumes the following declarations:

```
NCTYPE_STATUS      status;
NCTYPE_OBJH        objh;
NCTYPE_BAUD_RATE   baudrate;
```

Get the value of an object's baud rate attribute.

```
status = ncGetAttribute(objh, NC_ATTR_BAUD_RATE,
sizeof(baudrate), &baudrate);
```


ncOpenObject

Purpose

Open an object.

Format

LabVIEW



C

```
NCTYPE_STATUS      ncOpenObject(NCTYPE_STRING ObjName,
                                NCTYPE_OBJH_P ObjHandlePtr)
```

Input

ObjName ASCII name of the object to open.

Output

ObjHandlePtr Object handle you use with all subsequent NI-CAN function calls. For C, the object handle is returned to you using the pointer ObjHandlePtr. For LabVIEW, the object handle is returned to you in ObjHandle out.

Description

ncOpenObject takes the name of an object to open and returns a handle to that object that you use with subsequent NI-CAN function calls.

ncOpenObject also initiates a cable detection test and reports any configuration errors for the new PCMCIA-CAN cards that support all types of National Instruments PCMCIA-CAN cables. If ncConfig is called before ncOpenObject, the cable detection is done at the ncConfig call time.

You can use two syntax schemes can used for ObjName: the object hierarchy syntax and the user-defined alias syntax.

Use the object hierarchy syntax to open any object supported by NI-CAN. The object hierarchy syntax specifies the complete hierarchy of an object so that NI-CAN knows both which object to open and where that object is located. This syntax consists of a list of one or more objects in the NI-CAN object hierarchy, each separated by a double colon.

When more than one object is required, any number of blanks can exist before or after the double colon.

Specify objects in the NI-CAN hierarchy using a class name followed by an instance number. The class name is a string of letters that describes the class to which the object belongs. Class names are not case-sensitive. The instance number is a numeric value that indicates which object of a class is being specified. Instance numbers are normally specified in decimal notation. If hexadecimal notation is desired, the number must be preceded by “0x,” as in the C programming language. For more information on NI-CAN object names, refer to Chapter 3, *NI-CAN Objects*.

The second scheme you can use for `ObjName` is that of user-defined aliases. You create a user-defined alias with the NI-CAN Configuration utility for use as an alias to a complete object hierarchy.

The syntax for user-defined aliases consists of a single ASCII name preceded by ‘#’. The ‘#’ character differentiates user-defined aliases from the predefined names of the object hierarchy.

Although NI-CAN can generally be used by multiple applications simultaneously, it does not allow more than one application to open the same object. For example, if one application opens `CAN0`, and another application attempts to open `CAN0`, the second `ncOpenObject` returns the error `NC_ERR_ALREADY_OPEN`. It is legal for one application to open `CAN0 : :STD14` and another application to open `CAN0 : :STD21`, because the two objects are considered distinct.

If `ncOpenObject` is successful, a handle to the newly opened object is returned. You use this object handle for all subsequent function calls for the object.

CAN Network Interface Object

For information on the `ObjName` of the CAN Network Interface Object, refer to the *CAN Network Interface Object* section of Chapter 3, *NI-CAN Objects*.

CAN Object

For information on the `ObjName` of the CAN Object, refer to the *CAN Object* section of Chapter 3, *NI-CAN Objects*.

Return Status

<code>NC_SUCCESS</code>	Success (no warning or error).
<code>NC_ERR_BAD_NAME</code>	Invalid or unrecognized name in <code>ObjName</code> .
<code>NC_ERR_BAD_PARAM</code>	Invalid parameter.
<code>NC_ERR_ALREADY_OPEN</code>	Object already opened by another application.
<code>NC_ERR_DRIVER</code>	Implementation-specific error in the NI-CAN driver.

Examples

These examples assume the following declarations:

```
NCTYPE_STATUS      status;  
NCTYPE_OBJH        objh;
```

1. Open a CAN Network Interface Object.

```
status = ncOpenObject ("CAN0", &objh);
```

2. Open a CAN Object at standard arbitration ID 14 on CAN1

```
status = ncOpenObject ("CAN1::STD14", &objh);
```

3. Open CAN object at extended arbitration ID 2043 hex on CAN2

```
status = ncOpenObject ("CAN2::XTD0x2043", &objh);
```

4. Open an alias to the CAN Object at standard arbitration ID 14 on CAN1. This alias was specified within the NI-CAN Configuration utility.

```
status = ncOpenObject ("#EngineSpeed", &objh);
```

5. This call returns an error of `NC_ERR_BAD_NAME` with qualifier 2 (80020003 hex), because the Z makes the CAN Object name invalid.

```
status = ncOpenObject ("CAN0::ZTD5", &objh);
```


ncRead

Purpose

Read the data value of an object.

Format

LabVIEW

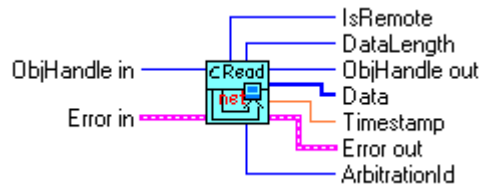

C

```
NCTYPE_STATUS ncRead(NCTYPE_OBJH ObjHandle,
NCTYPE_UINT32 DataSize,
NCTYPE_ANY_P DataPtr)
```

Input

ObjHandle
DataSize

Object handle.
Size of the data in bytes (C only).

Output

DataPtr

Data read from object. For C, the data is returned to you using the pointer `DataPtr`. For LabVIEW, the data is returned to you using object-specific output terminals.

Description

`ncRead` reads the data value of the object specified by `ObjHandle`.

For C, `DataPtr` points to the variable that holds the data. Its type is undefined so that you can use the appropriate host data type. `DataSize` indicates the size of variable pointed to by `DataPtr`, and is used to verify that the size you have available is compatible with the configured read size for the object.

For LabVIEW, the data is returned to you using object-specific output terminals.

You use `ncRead` to obtain data from the read queue of an object. Because NI-CAN handles the read queue in the background, this function does not wait for new data to arrive. To ensure that new data is available before calling `ncRead`, first wait for the `NC_ST_READ_AVAIL` state. The `NC_ST_READ_AVAIL` state transitions from false to true when NI-CAN places a new data item into an empty read queue, and remains true until you read the last data item from the queue.

When you call `ncRead` for an empty read queue (`NC_ST_READ_AVAIL` false), the data from the previous call to `ncRead` is returned to you again, along with the `NC_ERR_OLD_DATA` warning. If no data item has yet arrived for the read queue, a default data item is returned, which consists of all zeros.

When a new data item arrives for a full queue, NI-CAN discards the item, and the next call to `ncRead` returns the `NC_ERR_OVERFLOW` error, along with the qualifier `NC_QUAL_OVFL_READ`. You can avoid this overflow behavior by setting the read queue length to zero. When a new data item arrives for a zero length queue, it simply overwrites the previous item without indicating an overflow. The `NC_ST_READ_AVAIL` state and `NC_ERR_OLD_DATA` warning still behave as usual, but you can ignore them if you only want the most recent data. You can use the `NC_ATTR_READ_Q_LEN` attribute to configure the read queue length.

The host data type returned from `ncRead` is different for each NI-CAN object class. This type normally includes data received from the network along with a timestamp of when that data arrived.

For C, the timestamp that `ncRead` returns is an unsigned 64-bit integer compatible with the Win32 `FILETIME` type. When data arrives from the network and is placed in the read queue, NI-CAN obtains this timestamp from the absolute time attribute (`NC_ATTR_ABS_TIME`) of the CAN Network Interface Object. This absolute time is kept in a Coordinated Universal Time (UTC) format, the standard used for global timekeeping (times that are not specific to local time zone considerations). UTC-based time is loosely defined as the current date and time of day in Greenwich, England. Microsoft defines its UTC time (`FILETIME`) as a 64-bit counter of 100 ns intervals that have elapsed since 12:00 a.m., January 1, 1601. Because the timestamp returned by `ncRead` is compatible with `FILETIME`, you can pass it into the Win32 `FileTimeToLocalFileTime` function to convert it to your local time zone format, then pass

the resulting local time to the Win32 `FileTimeToSystemTime` function to convert it to the Win32 `SYSTEMTIME` type (a structure with fields for year, month, day, and so on). For more information on Win32 time types and functions, refer to the Win32 Software Development Kit (SDK) online help.

For LabVIEW, the timestamp that `ncRead` returns is compatible with the LabVIEW time format. LabVIEW time is a double-precision floating-point number (DBL) representing the number of seconds that have elapsed since 12:00 a.m., Friday, January 1, 1904, Coordinated Universal Time (UTC). You can pass this timestamp into LabVIEW time functions such as `Seconds To Date/Time`. You can also display the time in a numeric indicator of type DBL by using **Format & Precision** from the front panel to change from `Numeric` to `Time & Date` format (set **Seconds Precision** to 3 to display milliseconds). For more information, refer to the LabVIEW Online Reference.

CAN Network Interface Object

The host data type you use with `ncRead` is `NCTYPE_CAN_FRAME_TIMED`. For LabVIEW, each field of `NCTYPE_CAN_FRAME_TIMED` is returned in a terminal of the NI-CAN Read CAN Network Interface Object function (`ncReadNet.vi`). For C, `NCTYPE_CAN_FRAME_TIMED` is a structure. Table 2-4 describes the fields of `NCTYPE_CAN_FRAME_TIMED`.

Table 2-4. `NCTYPE_CAN_FRAME_TIMED` Field Names

Field Name	Data Type	Description
Timestamp	<code>NCTYPE_ABS_TIME</code>	Holds value of absolute timer (<code>NC_ATTR_ABS_TIME</code>) when frame was received.
ArbitrationId	<code>NCTYPE_CAN_ARBID</code>	CAN arbitration ID received with frame. For more information on how standard and extended arbitration IDs are encoded, refer to Chapter 1, <i>NI-CAN Host Data Types</i> .

Table 2-4. NCTYPE_CAN_FRAME_TIMED Field Names (Continued)

Field Name	Data Type	Description
IsRemote	NCTYPE_BOOL	Indicates whether frame is CAN remote frame (NC_TRUE) or CAN data frame (NC_FALSE). It is always false for ncRead, indicating a CAN data frame. The CAN Network Interface Object cannot receive incoming CAN remote frames. For low-speed CAN, this field holds a special value indicating low speed communication errors. For more information, refer to the description of the NC_ATTR_LOG_COMM_ERRORS attribute in the <i>CAN Network Interface Object</i> section of Chapter 3, <i>NI-CAN Objects</i> .
DataLength	NCTYPE_UINT8	Number of data bytes in frame.
Data	Array of bytes (NCTYPE_UINT8)	This array holds data bytes (8 maximum).

When a CAN frame arrives from over the network, NI-CAN first checks it for handling by an open CAN Object. If no CAN Object applies, NI-CAN filters the arbitration ID of the frame using the appropriate comparator and mask. If the frame is acceptable, NI-CAN places it into an available entry in the read queue of the CAN Network Interface Object.

CAN Object

The host data type you use with ncRead is NCTYPE_CAN_DATA_TIMED. For LabVIEW, each field of NCTYPE_CAN_DATA_TIMED is returned in a terminal of the NI-CAN Read CAN Object function (ncReadObj.vi). For C, NCTYPE_CAN_DATA_TIMED is a structure. Table 2-5 describes the fields of NCTYPE_CAN_DATA_TIMED.

Table 2-5. NCTYPE_CAN_DATA_TIMED Field Names

Field Name	Data Type	Description
Timestamp	NCTYPE_ABS_TIME	Holds value of absolute timer (NC_ATTR_ABS_TIME) when CAN data frame was received.
Data	Array of bytes (NCTYPE_UINT8)	Data bytes for CAN Object. Available only when CAN Object is configured to receive data. Length of Data is preconfigured using NC_ATTR_CAN_DATA_LENGTH attribute.

Return Status

NC_SUCCESS	Success (no warning or error).
NC_ERR_BAD_PARAM	Invalid parameter.
NC_ERR_DRIVER	Implementation-specific error in the NI-CAN driver.
NC_ERR_OLD_DATA	Data returned from ncRead is the same as the data returned from the previous call to ncRead.
NC_ERR_OVERFLOW	Read queue overflow. This error code does not apply to ncRead itself, but indicates an error in background communication. A valid data value is still returned to you from ncRead, and all other data received prior to the overflow remains in the read queue.
NC_ERR_TIMEOUT	Watchdog timeout expired for a CAN Object. This error code does not apply to ncRead itself, but indicates an error in background communication.
NC_ERR_CAN_BUS_OFF	Error or warning indicating CAN communication errors. This error code does not apply to ncRead itself, but indicates an error in background communication.

Examples

These examples assume the following declarations:

```
NCTYPE_STATUS      status;
NCTYPE_OBJH        objh;
NCTYPE_CAN_FRAME_TIMED rframe;
NCTYPE_CAN_DATA_TIMED rdata;
```

1. Read from a CAN Network Interface Object.

```
status = ncRead(objh, sizeof(rframe), &rframe);
```
2. Read from a CAN Object.

```
status = ncRead(objh, sizeof(rdata), &rdata);
```


ncReadMult

Purpose

Read multiple data values from an object's queue.

Format

LabVIEW

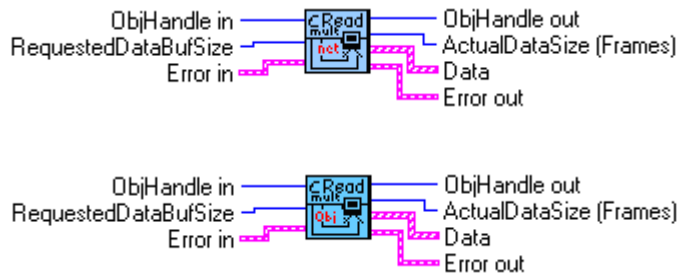

C

```
NCTYPE_STATUS ncReadMult (NCTYPE_OBJH ObjHandle,
                          NCTYPE_UINT32 DataSize,
                          NCTYPE_ANY_P DataPtr,
                          NCTYPE_UINT32_P ActualDataSize);
```

Input

ObjHandle	Object handle.
DataSize	Size of the data buffer in bytes (C only)
DataPtr	For C, points to data buffer in which the data returned. For LabVIEW, the data returned in object-specific output terminals.

Output

ActualDataSize	Number of bytes actually dequeued
----------------	-----------------------------------

Description

This function returns multiple data points from the read queue of the object specified by ObjHandle. When used with the Network Interface, ncReadMult is useful in analyzer applications where data frames need to be acquired at a high speed and stored for analysis in the future. For single frame and most recent data frame acquisition, you should use ncRead.

For C, `DataPtr` points to the variable that holds the data. Its type is undefined so that you can use the appropriate host data type. `DataSize` indicates the size of variable pointed to by `DataPtr`, and is used to verify that the size you have available is compatible with the configured read size for the object.

For LabVIEW, the data is returned to you using object-specific output terminals.

`DataSize` is the size of the buffer (array) that will hold the data. This buffer must be of the appropriate host data type. The buffer size (in terms of host data type) should be less than or equal to the Read Queue Length that you have setup for the particular object. `DataPtr` points to the first element of the data buffer and can be of type void or a pointer to the host data type being used (refer to `nican.h` for a list of host data types and their associated pointer types). For more information on the host data type returned, refer to the `ncRead` function.

Because NI-CAN handles the read queue in the background, this function does not wait for new data to arrive. To ensure that new data is available before calling `ncReadMult`, first wait for the `NC_ST_READ_AVAIL` state. Refer to the `ncRead` function for more information on this state.

This function does not return any old data for an empty queue or `NC_ERR_OLD_DATA` warnings. If there is no new data, the function returns with an `ActualDataSize` of zero.

The description for `NC_ERR_OVERFLOW`, host data types, and return status is identical to that of `ncRead` with the exception of `NC_ERR_OLD_DATA`, described above.

Refer to the `ncRead` function description for more details on the structures/clusters used with the CAN Network Interface Object and timestamps.

Return Status

<code>NC_SUCCESS</code>	Success (no warning or error)
<code>NC_ERR_BAD_PARAM</code>	Invalid parameter
<code>NC_ERR_DRIVER</code>	Implementation-specific error in the NI-CAN driver
<code>NC_ERR_OVERFLOW</code>	Read queue overflow. This error code does not apply to <code>ncReadMult</code> itself, but indicates an error in background communication. A valid data value is still returned to you from <code>ncReadMult</code> , and all other data received prior to the overflow remains in the read queue.
<code>NC_ERR_TIMEOUT</code>	Watchdog timeout expired for a CAN Object. This error code does not apply to <code>ncReadMult</code> itself, but indicates an error in background communication.
<code>NC_ERR_CAN_BUS_OFF</code>	Error or warning indicating CAN communication errors. This error code does not apply to <code>ncReadMult</code> itself, but indicates an error in background communication.

Examples

These examples assume the following declarations:

```
NCTYPE_STATUS      Status;
NCTYPE_OBJH        Rxhandle;
```

1. Read from Network Interface Object:

```
NCTYPE_CAN_FRAME_TIMED  ReceiveBuf[140]; //buffer of 140 frames
NCTYPE_UINT32           ActualDataSize;
NCTYPE_CAN_FRAME_TIMED_P RecvPtr;
RecvPtr = ReceiveBuf;
Status = ncReadMult(RxHandle, sizeof(ReceiveBuf), RecvPtr,
                   &ActualDataSize);
.
.
ActualDataSize = ActualDataSize/sizeof(NC_TYPE_CAN_FRAME_TIMED);
```

2. Read from CAN Object:

```
NCTYPE_CAN_DATA_TIMED   ReceiveBuf[140]; //buffer of 140 frames
NCTYPE_CAN_DATA_TIMED   Recv;
NCTYPE_UINT32           ActualDataSize;
NCTYPE_CAN_DATA_TIMED_P RecvPtr;
RecvPtr = ReceiveBuf;
Status = ncReadMult(RxHandle, sizeof(ReceiveBuf), RecvPtr,
                   &ActualDataSize);
.
.
ActualDataSize = ActualDataSize/sizeof(NCTYPE_CAN_DATA_TIMED);
```

ncReset

Purpose

Reset the board

Format

LabVIEW



C

```
NCTYPE_STATUS _NCFUNC_ncReset(NCTYPE_STRING IntfName, NCTYPE_UINT32
    Param);
```

Input

IntfName	Interface name (example: CAN0)
Param	Reserved for future use (set to 0)

Description

This function completely resets the CAN interface and ensures that all handles for that interface are closed.

If an NI-CAN application is terminated prior to closing all handles, the `NC_ERR_NOT_STOPPED` or `NC_ERR_ALREADY_OPEN` error might occur when the application is restarted. This often occurs in LabVIEW when the toolbar **Stop** button is used, or when a wiring problem with `ObjHandle` exists.

By making this the first NI-CAN function called in your application (preceding all `ncConfig`), you can avoid problems related to improper termination.

You can only use the `ncReset` function if you plan to run a single NI-CAN application. If you run more than one NI-CAN application, each with `ncReset`, the second `ncReset` call will close all handles for the first application.

You should only use the `ncReset` function as a temporary measure. After you update your application so that it successfully closes NI-CAN handles on termination, it should no longer be used.


ncSetAttribute

Purpose

Set the value of an object's attribute.

Format

LabVIEW



C

```
NCTYPE_STATUS ncSetAttribute(NCTYPE_OBJH ObjHandle,
NCTYPE_ATTRID AttrId,
NCTYPE_UINT32 AttrSize,
NCTYPE_ANY_P AttrPtr)
```

Input

ObjHandle	Object handle.
AttrId	Identifier of the attribute to set.
AttrSize	Size of the attribute in bytes (C only).
AttrPtr (AttrValue)	New attribute value. For C, you provide the attribute value using the pointer AttrPtr. For LabVIEW, you provide the attribute value in AttrValue.

Description

ncSetAttribute sets the value of the attribute specified by AttrId in the object specified by ObjHandle. ncSetAttribute can be used only for attributes with Set permissions, not Get (ncGetAttribute only) or Config (ncConfig only).

For C, AttrPtr points to the variable that holds the attribute value. Its type is undefined so that you can use the appropriate host data type for AttrId. AttrSize indicates the size of variable pointed to by AttrPtr.

For LabVIEW, this function sets the value of an object's attribute using a LabVIEW U32 (AttrValue), so a size is not needed.

CAN Network Interface Object

For information on the attributes of the CAN Network Interface Object, refer to the [CAN Network Interface Object](#) section of Chapter 3, *NI-CAN Objects*.

CAN Object

For information on the attributes of the CAN Object, refer to the [CAN Object](#) section of Chapter 3, *NI-CAN Objects*.

Return Status

NC_SUCCESS	Success (no error or warning).
NC_ERR_BAD_PARAM	Invalid parameter. This error is returned when the attribute specified by <code>AttrId</code> has <code>Get</code> or <code>Config</code> permissions.
NC_ERR_BAD_VALUE	The value of the attribute is invalid for the specified <code>AttrId</code> .
NC_ERR_DRIVER	Implementation-specific error in the NI-CAN driver.

Example

This example assumes the following declarations:

```
NCTYPE_STATUS      status;
NCTYPE_OBJH        objh;
NCTYPE_ABS_TIME    abstime;
```

Set the absolute time to zero.

```
abstime.LowPart = 0;
abstime.HighPart = 0;
status = ncSetAttribute(objh, NC_ATTR_ABS_TIME,
sizeof(abstime), &abstime);
```


ncWaitForState

Purpose

Wait for one or more states to occur in an object.

Format

LabVIEW



C

```
NCTYPE_STATUS      ncWaitForState(NCTYPE_OBJH ObjHandle,
                                NCTYPE_STATE DesiredState,
                                NCTYPE_DURATION Timeout,
                                NCTYPE_STATE_P StatePtr)
```

Input

ObjHandle	Object handle.
DesiredState	States to wait for (bitmask).
Timeout	Length of time to wait.

Output

StatePtr (State)	Current state of object when desired states occur. For C, the state is returned to you using the pointer StatePtr. For LabVIEW, the state is returned to you in State.
------------------	------------------------------------------------------------------------------------------------------------------------------------------------------------------------

Description

You use `ncWaitForState` to wait for one or more states to occur in the object specified by `ObjHandle`.

This function waits up to `Timeout` for one of the bits set in `DesiredState` to become set in the attribute `NC_ATTR_STATE`. You can use the special `Timeout` value `NC_DURATION_INFINITE` (FFFFFFFF hex) to wait indefinitely.

When the states in `DesiredState` are detected, the function returns the current value of the `NC_ATTR_STATE` attribute. If an error occurs, the state returned is zero.

While waiting for the desired states, `ncWaitforState` suspends the current execution. For C, other Win32 threads in your application can still execute. For LabVIEW, functions that are not directly connected to `ncWaitforState` can execute.

If you want to allow other code in your application to execute while waiting for NI-CAN states, refer to the `ncCreateNotification` (C only) and `ncCreateOccurrence` (LabVIEW only) functions.

Return Status

<code>NC_SUCCESS</code>	Success (no error or warning).
<code>NC_ERR_BAD_PARAM</code>	Invalid parameter.
<code>NC_ERR_TIMEOUT</code>	Timeout expired before any desired states occurred.
<code>NC_ERR_DRIVER</code>	Implementation-specific error in the NI-CAN driver.

Examples

These examples assume the following declarations:

```
NCTYPE_STATUS      status;
NCTYPE_OBJH        objh;
NCTYPE_STATE       state;
```

1. Wait no more than 10 seconds for data to arrive in the read queue.

```
status = ncWaitforState(objh, NC_ST_READ_AVAIL, 10000, &state);
```

2. Wait no more than 100 milliseconds for a previous `ncWrite` to succeed, or for a background warning/error, such as bus off, to occur.

```
status = ncWaitforState(objh, (NC_ST_WRITE_SUCCESS | NC_ST_WARNING
| NC_ST_ERROR), 100, &state);
```



ncWrite

Purpose

Write the data value of an object.

Format

LabVIEW

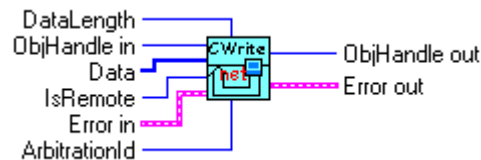

C

```
NCTYPE_STATUS ncWrite(NCTYPE_OBJH ObjHandle,
NCTYPE_UINT32 DataSize,
NCTYPE_ANY_P DataPtr)
```

Input

ObjHandle	Object handle.
DataSize	Size of the data in bytes.
DataPtr	Data written to the object. For C, you provide the data using the pointer <code>DataPtr</code> . For LabVIEW, you provide the data using object-specific input terminals.

Description

`ncWrite` writes the data value of the object specified by `ObjHandle`.

For C, `DataPtr` points to the variable from which the data is written. Its type is undefined so that you can use the appropriate host data type. `DataSize` indicates the size of variable pointed to by `DataPtr`, and is used to verify that the size you provide is compatible with the configured write size for the object.

For LabVIEW, you provide the data using object-specific input terminals.

You use `ncWrite` to place data into the write queue of an object. Because NI-CAN handles the write queue in the background, this function does not wait for data to be transmitted on the network. To make sure that the data is transmitted successfully after calling `ncWrite`, wait for the `NC_ST_WRITE_SUCCESS` state. The `NC_ST_WRITE_SUCCESS` state transitions from false to true when the write queue is empty, and NI-CAN has successfully transmitted the last data item onto the network. The `NC_ST_WRITE_SUCCESS` state remains true until you write another data item into the write queue.

When you configure an object to transmit data onto the network periodically, it obtains data from the object's write queue each period. If the write queue is empty, NI-CAN transmits the data of the previous period again. NI-CAN transmits this data repetitively until the next call to `ncWrite`.

If an object's write queue is full, a call to `ncWrite` returns the `NC_ERR_OVERFLOW` error (along with qualifier `NC_QUAL_OVFL_WRITE`), and NI-CAN discards the data you provide. One way to avoid this overflow error is to set the write queue length to zero. When `ncWrite` is called for a zero length queue, the data item you provide with `ncWrite` simply overwrites the previous data item without indicating an overflow. A zero length write queue is often useful when an object is configured to transmit data onto the network periodically, and you simply want to transmit the most recent data value each period. It is also useful when you plan to always wait for `NC_ST_WRITE_SUCCESS` after every call to `ncWrite`. You can use the `NC_ATTR_WRITE_Q_LEN` attribute to configure the write queue length.

The host data type you provide to `ncWrite` is different for each NI-CAN object class.

CAN Network Interface Object

The host data type you use with `ncWrite` is `NCTYPE_CAN_FRAME`. For LabVIEW, each field of `NCTYPE_CAN_FRAME` is provided in a terminal of the NI-CAN Write CAN Network Interface Object function (`ncWriteNet.vi`). For C, `NCTYPE_CAN_FRAME` is a structure. Table 2-6 describes the fields of `NCTYPE_CAN_FRAME`.

Table 2-6. NCTYPE_CAN_FRAME Field Names

Field Name	Data Type	Description
ArbitrationId	NCTYPE_CAN_ARBITID	CAN arbitration ID to transmit with frame. For information on how standard and extended arbitration IDs are encoded, refer to Chapter 1, <i>NI-CAN Host Data Types</i> .
IsRemote	NCTYPE_BOOL	Indicates whether frame is CAN remote frame (<code>NC_TRUE</code>) or CAN data frame (<code>NC_FALSE</code>).

Table 2-6. NCTYPE_CAN_FRAME Field Names (Continued)

Field Name	Data Type	Description
DataLength	NCTYPE_UINT8	When <code>IsRemote</code> is false, this field specifies number of data bytes in frame. When <code>IsRemote</code> is true, it specifies desired number of data bytes.
Data	Array of bytes (NCTYPE_UINT8)	When <code>IsRemote</code> is false, this array holds data bytes (8 maximum).

Sporadic, recoverable errors on the CAN network interface are handled automatically by the protocol, and are not reported as errors from NI-CAN. As such, after `ncWrite` returns successfully, NI-CAN eventually transmits the frame on the CAN network unless the `NC_ERR_CAN_BUS_OFF` warning occurs.

CAN Object

The host data type you use with `ncWrite` is `NCTYPE_CAN_DATA`. For LabVIEW, each field of `NCTYPE_CAN_DATA` is provided in a terminal of the NI-CAN Write CAN Object function (`ncWriteObj.vi`). For C, `NCTYPE_CAN_DATA` is a structure.

For CAN Objects configured to transmit a CAN remote frame when you call `ncWrite` (Receive Value with Call), you do not provide data to `ncWrite`. For C, you set `DataSize` to zero. For LabVIEW, you leave the `Data` terminal of `ncWriteObj.vi` unconnected. For more information on Receive Value with Call, refer to the description of the `NC_ATTR_COMM_TYPE` attribute.

Table 2-7 describes the field of `NCTYPE_CAN_DATA`.

Table 2-7. NCTYPE_CAN_DATA Field Name

Field Name	Data Type	Description
Data	Array of bytes (NCTYPE_UINT8)	Data bytes for CAN Object. Available only when CAN Object is configured to transmit data. Length of <code>Data</code> is preconfigured using <code>NC_ATTR_CAN_DATA_LENGTH</code> attribute.

Return Status

<code>NC_SUCCESS</code>	Success (no error or warning).
<code>NC_ERR_BAD_PARAM</code>	Invalid parameter.
<code>NC_ERR_DRIVER</code>	Implementation-specific error in the NI-CAN driver.
<code>NC_ERR_OVERFLOW</code>	Write queue overflow. This error occurs when the write queue of the object is full, and the data value you provided cannot be

<code>NC_ERR_TIMEOUT</code>	queued for later transmission. The error can occur only if the write queue length (<code>NC_ATTR_WRITE_Q_LEN</code>) is nonzero. Watchdog timeout expired for a CAN Object. This error code does not apply to <code>ncWrite</code> itself, but indicates an error in background communication.
<code>NC_ERR_CAN_BUS_OFF</code>	Error or warning indicating CAN communication errors. This error code does not apply to <code>ncWrite</code> itself, but indicates an error in background communication.

Examples

These examples assume the following declarations:

```
NCTYPE_STATUS      status;
NCTYPE_OBJH        objh;
NCTYPE_CAN_FRAME_TIMED wframe;
NCTYPE_CAN_DATA_TIMED wdata;
```

1. Write to a CAN Network Interface Object.

```
status = ncWrite(objh, sizeof(wframe), &wframe);
```

2. Write to a CAN Object.

```
status = ncWrite(objh, sizeof(wdata), &wdata);
```

NI-CAN Objects

This chapter lists the syntax of the `ObjName` for each object class, specifies what the object encapsulates, and gives an overview of the major features and uses of each object.

For information on how each NI-CAN function is used with the following object classes, refer to Chapter 2, *NI-CAN Functions*.

Object Names

The objects in this chapter are listed in alphabetical order. For each object class, the syntax of its `ObjName` is discussed.

Encapsulates

Each object description includes a brief summary of what the object encapsulates.

Description

The description section gives an overview of the major features and uses of the object.

Attributes

The attributes section lists and describes the attributes for each object. The attributes are listed in alphabetical order.

For each attribute, the description lists its host data type, its attribute ID, and its permissions. Attribute permissions consist of one of the following:

<code>Get</code>	You can get the attribute at any time, but never set it.
<code>Set</code>	You can get or set the attribute at any time.
<code>Config</code>	You can get the attribute at any time, but you can set it only by using the <code>ncConfig</code> function. These attributes are called configuration attributes. NI-CAN obtains the initial value of configuration attributes from the NI-CAN Configuration utility, and you can override them only by using <code>ncConfig</code> , not <code>ncSetAttribute</code> .

CAN Network Interface Object

Object Name

CAN x

The letters CAN indicate the class of the CAN Network Interface Object, and x is a decimal number starting at zero that indicates which CAN network interface is being referenced (CAN0, CAN1, and so on). Use the NI-CAN Configuration utility to associate instance numbers with physical network interface ports.

Encapsulates

CAN network interface.

Description

The CAN Network Interface Object encapsulates a physical interface to a CAN network, usually a CAN port on an AT, PCI, or PCMCIA interface.

The communication facilities of the CAN Network Interface Object basically consist of a read queue and a write queue. You use the `ncRead` function to read CAN frames from the read queue in the order they arrive. When an incoming frame arrives, the `NC_ST_READ_AVAIL` state sets, to notify you that one or more CAN frames are in the read queue. You use the `ncWrite` function to write CAN frames to the write queue. NI-CAN transmits CAN frames from the write queue in the order written. When all CAN frames in the write queue are transmitted successfully, the `NC_ST_WRITE_SUCCESS` state sets.

You can use the CAN Network Interface Object for communication along with CAN Objects. When one or more CAN Objects are open, the CAN Network Interface Object cannot receive frames that would normally be handled by the CAN Objects. For example, if you open the CAN Object named `CAN0::STD5`, then the CAN Network Interface Object cannot receive frames with standard arbitration ID 5.

If you choose not to configure the CAN Network Interface Object to start automatically (`NC_ATTR_START_ON_OPEN` attribute is false), it opens in the stopped state (not communicating). To start network communication for the CAN Network Interface Object and all higher level CAN Objects, call `ncAction` with `NC_OP_START`. You might want to do this when you have an application that tests an installed CAN network. In this sort of environment, you would load test patterns (lists of data values) into various write queues, then use `NC_OP_START` to start the test sequence.

Error Active, Error Passive, and Bus Off States

The CAN communication controller used by NI-CAN network interfaces is the Intel 82527. Although this chip provides no direct means of detecting the error passive state, it can detect when one of its error counters increments above 96. When this occurs, NI-CAN sets the `NC_ST_WARNING` state in the `NC_ATTR_STATE` attribute of the CAN Network Interface Object and all of its higher level CAN Objects. The background status attribute (`NC_ATTR_STATUS`) is set with the status code `NC_ERR_CAN_BUS_OFF` and a warning severity.

When the transmit error counter of the Intel 82527 increments above 255, the network interface transfers into the bus off state as dictated by the CAN protocol. The network interface stops communication so that you can correct the defect in the network, such as a malfunctioning cable or device. When bus off occurs, the `NC_ST_ERROR` and `NC_ST_STOPPED` states are set in the `NC_ATTR_STATE` attribute of the CAN Network Interface Object and all of its higher level CAN Objects. The background status attribute (`NC_ATTR_STATUS`) is set with the status code `NC_ERR_CAN_BUS_OFF` and an error severity.

Whether the severity of `NC_ERR_CAN_BUS_OFF` is a warning or error, the status qualifier is set to indicate the most recently detected communications error. This qualifier can have the value `NC_QUAL_CAN_STUFF` (more than five equal bits), `NC_QUAL_CAN_FORM` (wrong frame format), `NC_QUAL_CAN_ACK` (frame not acknowledged), `NC_QUAL_CAN_BIT1` (transmitted one but detected zero), `NC_QUAL_CAN_BIT0`, or `NC_QUAL_CAN_CRC` (wrong CRC checksum). Refer to the CAN protocol specification for a complete description of these communication errors.

If no CAN devices are connected to the network interface port, and you attempt to transmit a frame, the `NC_ERR_CAN_BUS_OFF` status occurs with a warning severity. This warning occurs because the missing acknowledgment bit increments the transmit error counter until the network interface reaches the error passive state, but bus off state is never reached.

Because the error counters in the CAN chip reflect the status of the CAN network, and not necessarily your CAN application, a given `NC_ERR_CAN_BUS_OFF` warning will often remain from one run of your application to the next. If you want to clear the CAN chip's error counters (and the `NC_ERR_CAN_BUS_OFF` warning) completely when your application starts, use `ncAction` of `NC_OP_RESET` to reset the CAN chip, then use `ncAction` of `NC_OP_START` to resume communication.

For more information about low-speed communication error handling, refer to the description of the `NC_ATTR_LOG_COMM_ERRS` attribute in the *CAN Network Interface Object* section of this chapter.

Attributes

NC_ATTR_ABS_TIME (Absolute Time)

Attribute ID	NC_ATTR_ABS_TIME
Hex Encoding	80000008
Data Type	NC_ATTR_ABS_TIME
Permissions	Set
Description	<p>Absolute time of the network interface. The NI-CAN driver uses this attribute for timestamps returned by <code>ncRead</code>. When the NI-CAN driver first initializes (for example, when the host computer is powered on), it is set to the system time of the host computer, and thus keeps the absolute time since that point. You can set this attribute to zero to keep absolute time from a given point, but then the <code>ncRead</code> timestamp is no longer compatible with Win32 FILETIME or LabVIEW time. For more information, refer to the description of the <code>ncRead</code> function in Chapter 2, <i>NI-CAN Functions</i>.</p> <p>This attribute applies to all objects of the CAN network interface hardware product. For example, if an interface board contains two network interface ports, this attribute applies to both CAN Network Interface Objects.</p>

NC_ATTR_BAUD_RATE (Baud Rate)

Attribute ID	NC_ATTR_BAUD_RATE
Hex Encoding	80000007
Data Type	NCTYPE_BAUD_RATE
Permissions	Config
Description	<p>Baud rate of the network interface. NI-CAN calculates values for various CAN timing parameters and programs them based on the baud rate. All common baud rates are supported, including 10 kb/s, 100 kb/s, 125 kb/s, 250 kb/s, 500 kb/s, and 1000 kb/s.</p>

NC_ATTR_CAN_COMP_STD (Standard Comparator)

Attribute ID	NC_ATTR_CAN_COMP_STD
Hex Encoding	80010001
Data Type	NCTYPE_CAN_ARBID
Permissions	Config
Description	<p>CAN arbitration ID for the standard frame comparator. This comparator filters all incoming standard (11-bit) CAN frames placed into the read queue. The NC_FL_CAN_ARBID_XTD bit must be clear for any value written to this attribute. For more information, refer to the description of NCTYPE_CAN_ARBID in Chapter 1, <i>NI-CAN Host Data Types</i>.</p> <p>If you intend to use CAN Objects as the sole means of receiving standard CAN frames from the network, you should disable all standard frame reception in the CAN Network Interface Object by setting this attribute to NC_CAN_ARBID_NONE (CFFFFFFF hex). With this setting, the network interface is best able to filter out all incoming standard CAN frames except those handled by the CAN Objects.</p>

NC_ATTR_CAN_COMP_XTD (Extended Comparator)

Attribute ID	NC_ATTR_CAN_COMP_XTD
Hex Encoding	80010003
Data Type	NCTYPE_CAN_ARBID
Permissions	Config
Description	<p>CAN arbitration ID to the extended frame comparator. This comparator filters all incoming extended (29-bit) CAN frames placed into the read queue. The NC_FL_CAN_ARBID_XTD bit must be set for any value written to this attribute. For more information, refer to the description of NCTYPE_CAN_ARBID in Chapter 1, <i>NI-CAN Host Data Types</i>.</p> <p>If you intend to use CAN Objects as the sole means of receiving extended CAN frames from the network, you should disable all extended frame reception in the CAN Network Interface Object by setting this attribute to NC_CAN_ARBID_NONE (CFFFFFFF hex). With this setting, the network interface is best able to filter out all incoming extended CAN frames except those handled by the CAN Objects.</p>

NC_ATTR_CAN_MASK_STD (Standard Mask)

Attribute ID	NC_ATTR_CAN_MASK_STD
Hex Encoding	80010002
Data Type	NCTYPE_UINT32
Permissions	Config
Description	<p>Bitmask used in conjunction with NC_ATTR_CAN_COMP_STD for filtration of incoming standard CAN frames. For each bit set in the mask, NI-CAN checks the corresponding bit in the standard frame comparator for a match. Bits in the mask that are clear are treated as don't-cares. For example, hex 000007FF means to compare all 11 bits of incoming standard CAN frames. If the standard frame comparator is NC_CAN_ARBID_NONE, NI-CAN ignores this mask, because all standard frame reception is disabled in the CAN Network Interface Object.</p>

NC_ATTR_CAN_MASK_XTD (Extended Mask)

Attribute ID	NC_ATTR_CAN_MASK_XTD
Hex Encoding	80010004
Data Type	NCTYPE_UINT32
Permissions	Config
Description	Bitmask used in conjunction with NC_ATTR_CAN_COMP_XTD for filtration of incoming extended CAN frames. For each bit set in the mask, NI-CAN checks the corresponding bit in the extended frame comparator for a match. Bits in the mask that are clear are treated as don't-cares. For example, hex 1FFFFFFF means to compare all 29 bits of incoming extended CAN frames. If the extended frame comparator is NC_CAN_ARBITID_NONE, NI-CAN ignores this mask.

NC_ATTR_PROTOCOL (Protocol)

Attribute ID	NC_ATTR_PROTOCOL
Hex Encoding	80000001
Data Type	NCTYPE_PROTOCOL
Permissions	Get
Description	Protocol implemented by the CAN Network Interface Object. The value is always NC_PROTOCOL_CAN (00000001 hex).

NC_ATTR_PROTOCOL_VERSION (Protocol Version)

Attribute ID	NC_ATTR_PROTOCOL_VERSION
Hex Encoding	80000002
Data Type	NCTYPE_VERSION
Permissions	Get
Description	Version that indicates the level of conformance to the protocol specification. The value is always hex 02000200 (major version 2, minor version 0, subminor B), to indicate conformity with CAN 2.0 Parts A and B. The CAN implementation under NI-CAN also complies with ISO 11898.

NC_ATTR_READ_PENDING (Read Entries Pending)

Attribute ID	NC_ATTR_READ_PENDING
Hex Encoding	80000011
Data Type	NCTYPE_UINT32
Permissions	Get
Description	Indicates the number of pending entries in the read queue. If NC_ATTR_READ_PENDING is zero, the NC_ST_READ_AVAIL state is clear.

NC_ATTR_READ_Q_LEN (Read Queue Length)

Attribute ID	NC_ATTR_READ_Q_LEN
Hex Encoding	80000013
Data Type	NCTYPE_UINT32
Permissions	Config
Description	Length (maximum number of entries) for the read queue. For more information, refer to the description of the ncRead function in Chapter 2, <i>NI-CAN Functions</i> .

NC_ATTR_SOFTWARE_VERSION (Software Version)

Attribute ID	NC_ATTR_SOFTWARE_VERSION
Hex Encoding	80000003
Data Type	NCTYPE_VERSION
Permissions	Get
Description	Version of the NI-CAN driver that implements this object as well as all objects above it in the object hierarchy. This is the National Instruments version number, not the version of the protocol.

NC_ATTR_START_ON_OPEN (Start On Open)

Attribute ID	NC_ATTR_START_ON_OPEN
Hex Encoding	80000006
Data Type	NCTYPE_BOOL
Permissions	Config
Description	Indicates whether communication starts for the CAN Network Interface Object (and all CAN Objects above it in the hierarchy) immediately after you open an object with <code>ncOpenObject</code> . You must always set this attribute within the NI-CAN Configuration utility. It is normally set to true after you use the utility to specify needed configuration attributes such as baud rate. When this attribute is set to true, NI-CAN starts communication transparently. When this attribute is set to false, you must use <code>ncAction</code> to issue <code>NC_OP_START</code> on the CAN Network Interface Object to begin network communication.

NC_ATTR_STATE (Object State)

Attribute ID	NC_ATTR_STATE
Hex Encoding	80000009
Data Type	NCTYPE_STATE
Permissions	Get
Description	Current state of the CAN network interface. For more information, refer to Appendix A, <i>NI-CAN Object States</i> .

NC_ATTR_STATUS (Object Status)

Attribute ID	NC_ATTR_STATUS
Hex Encoding	8000000A
Data Type	NCTYPE_STATUS
Permissions	Get
Description	Background status of the CAN network interface. Unless the NC_ST_WARNING or NC_ST_ERROR states are set in NC_ATTR_STATE, this attribute always returns NC_SUCCESS. When you read an error or warning from this attribute, NI-CAN clears the appropriate state and sets the background status back to NC_SUCCESS. Sporadic, recoverable errors on the CAN network interface are handled automatically by the protocol, and are not reported as errors from NI-CAN. If a background error occurs, you can read it from this attribute, or obtain it from the next call to ncRead or ncWrite.

NC_ATTR_WRITE_PENDING (Write Entries Pending)

Attribute ID	NC_ATTR_WRITE_PENDING
Hex Encoding	80000012
Data Type	NCTYPE_UINT32
Permissions	Get
Description	Indicates the number of pending entries in the write queue. If NC_ST_WRITE_PENDING is zero, the NC_ST_WRITE_SUCCESS state is set (after NI-CAN successfully transmits the final frame).

NC_ATTR_WRITE_Q_LEN (Write Queue Length)

Attribute ID	NC_ATTR_WRITE_Q_LEN
Hex Encoding	80000014
Data Type	NCTYPE_UINT32
Permissions	Config
Description	Length (maximum number of entries) for the write queue. For more information, refer to the description of the ncWrite function in Chapter 2, <i>NI-CAN Functions</i> .

NC_ATTR_RX_Q_LEN (Rx Queue Length)

Attribute ID	NC_ATTR_RX_Q_LEN
Hex Encoding	A0000004
Data Type	NCTYPE_UINT32
Permissions	Config
Description	<p>Sets the length of the onboard receive queue. This queue is a transitional queue between the CAN Controller and the actual read queue of the CAN Network Interface and/or CAN Object. The default length of this queue is 50.</p> <p>In certain high-traffic situations, you might receive an error status 0x80030008. This is an NC_ERR_OVERFLOW error that uses the following qualifier:</p> <pre>#define NC_QUAL_OVFL_RX_G 0X0030000</pre> <p>If you see this receive queue overflow error, increase the length to the maximum number of frames that you would expect to receive in a burst (back-to-back).</p>

NC_ATTR_LOG_COMM_ERRS (Low-Speed CAN)

Attribute ID	NC_ATTR_LOG_COMM_ERRS
Hex Encoding	8001000A
Data Type	NCTYPE_BOOL
Permissions	Config
Description	<p>This attribute only applies to low-speed CAN interfaces.</p> <p>If this CAN Network Interface attribute is set to <code>NC_TRUE</code> (by adding to the <code>ncConfig</code> list), CAN communication errors are logged to the interface read queue, and are not reported in NI-CAN status. When looking at a frame read using <code>ncRead</code>, a CAN communication error is detected by checking from the following special value in the <code>IsRemote</code> field of the <code>NCTYPE_CAN_FRAME_TIMED</code> structure:</p> <pre>#define NC_FRMTYPE_COMM_ERR 2</pre> <p>When <code>IsRemote</code> has this value, the <code>ArbitrationId</code> field holds a status value similar to the return value from an NI-CAN function. The <code>TimeStamp</code> field indicates the time when the error occurred (or cleared). This <code>ArbitrationId</code> field will consist of one of the following values:</p> <pre>0x4000000B-0x4006000B Bus off warning occurred (error passive) 0x8000000B-0x8006000B Bus off error occurred (bus off) 0x0000000B Bus off warning/error has cleared 0x8000000C Low-speed transceiver error detected 0x0000000C Low-speed transceiver error cleared</pre> <p>Note: The default value for this attribute is <code>NC_FALSE</code>.</p> <p>For LabVIEW, this attribute is configured using the Network Interface Config Cluster-LS and the <code>ncConfigCANNetLS.vi</code>.</p>

NC_ATTR_READ_MULT_SIZE (ReadMult Size for Notification)

Attribute Id	NC_ATTR_READ_MULT_SIZE
Hex Encoding	0x8001000B
Data Type	NCTYPE_UINT32
Permissions	Config, Set, Get
Description	<p>Sets the size (in number of frames) that NI-CAN will use to notify the user when specified amount of frames are available in the Read Queue. Once the application receives the notification, the user can call <code>ncReadMult</code> to read the desired number of frames. By using this functionality, a user does not need to poll the queue constantly to read frames.</p> <p>Note that the <code>ncCreateNotification</code> (or <code>ncCreateOccurance</code>) function must use a desired state of <code>NC_ST_READ_MULT</code> (hex encoding <code>0x00000008</code>).</p> <p>In LabVIEW, you can set the attribute by using the <code>ncSetAttribute</code> function after calling <code>ncConfig</code> and <code>ncOpen</code> for the object. The user then needs to call <code>ncCreateOccurance</code>, as shown in this manual, with the aforementioned state (<code>0x08</code>) as the Desired State.</p> <p>In C, you can do this by either adding it to the Network Interface attribute configuration or calling <code>ncSetAttribute</code> function. The function call to <code>ncCreateNotification</code> must have the Desired State of <code>NC_ST_READ_MULT</code>.</p>

NC_ATTR_RTSI_MODE (RTSI Mode)

Attribute Id	NC_ATTR_RTSI_MODE (RTSI Mode)
Hex Encoding	0x80000017
Data Type	NCTYPE_UINT32
Permissions	Config, Set

<p>Description</p>	<p>This attribute defines whether the user needs to configure the CAN object as an RTSI driver or the DAQ board as the RTSI driver. The following values can be used:</p> <p>Attribute values:</p> <table border="0"> <tr> <td>In C</td> <td>In LabVIEW RTSI Config Cluster</td> </tr> <tr> <td>NC_RTSI_NONE</td> <td>Disable RTSI</td> </tr> <tr> <td>NC_RTSI_TX_ON_IN</td> <td>On RTSI Input—Transmit CAN Frame</td> </tr> <tr> <td>NC_RTSI_TIME_ON_IN</td> <td>On RTSI Input—Timestamp RTSI event</td> </tr> <tr> <td>NC_RTSI_OUT_ON_RX</td> <td>RTSI Output on Receiving CAN Frame</td> </tr> <tr> <td>NC_RTSI_OUT_ON_TX</td> <td>RTSI Output on Transmitting CAN Frame</td> </tr> <tr> <td>NC_RTSI_OUT_ACTION_ONLY</td> <td>RTSI Output on ncAction call</td> </tr> </table> <p>Each mode is explained in detail below.</p> <p>NC_RTSI_TX_ON_IN (On RTSI Input-Transmit CAN Frame):</p> <p>In this mode, NI-CAN will transmit the most recent frame on an incoming RTSI trigger on the RTSI line configured via NC_ATTR_RTSI_SIGNAL. To begin transmission, a frame must be written to the write queue of the object (by calling ncWrite) and an RTSI signal applied to the configured RTSI line. NI-CAN will retransmit the last frame until a new frame is enqueued.</p> <p>NC_RTSI_TIME_ON_IN (On RTSI Input—Timestamp RTSI event):</p> <p>In this mode, NI-CAN will timestamp an incoming RTSI trigger on the RTSI line configured via NC_ATTR_RTSI_SIGNAL and enqueue in the object’s read queue a frame containing special entries in the following fields (as noted):</p> <table border="0"> <tr> <td>Timestamp:</td> <td>Time when RTSI event occurred</td> </tr> <tr> <td>Arbitration Id:</td> <td>0x40000001 (NC_FL_CAN_ARBID_INFO NC_ARBID_INFO_RTSI_INPUT)</td> </tr> </table>	In C	In LabVIEW RTSI Config Cluster	NC_RTSI_NONE	Disable RTSI	NC_RTSI_TX_ON_IN	On RTSI Input—Transmit CAN Frame	NC_RTSI_TIME_ON_IN	On RTSI Input—Timestamp RTSI event	NC_RTSI_OUT_ON_RX	RTSI Output on Receiving CAN Frame	NC_RTSI_OUT_ON_TX	RTSI Output on Transmitting CAN Frame	NC_RTSI_OUT_ACTION_ONLY	RTSI Output on ncAction call	Timestamp:	Time when RTSI event occurred	Arbitration Id:	0x40000001 (NC_FL_CAN_ARBID_INFO NC_ARBID_INFO_RTSI_INPUT)
In C	In LabVIEW RTSI Config Cluster																		
NC_RTSI_NONE	Disable RTSI																		
NC_RTSI_TX_ON_IN	On RTSI Input—Transmit CAN Frame																		
NC_RTSI_TIME_ON_IN	On RTSI Input—Timestamp RTSI event																		
NC_RTSI_OUT_ON_RX	RTSI Output on Receiving CAN Frame																		
NC_RTSI_OUT_ON_TX	RTSI Output on Transmitting CAN Frame																		
NC_RTSI_OUT_ACTION_ONLY	RTSI Output on ncAction call																		
Timestamp:	Time when RTSI event occurred																		
Arbitration Id:	0x40000001 (NC_FL_CAN_ARBID_INFO NC_ARBID_INFO_RTSI_INPUT)																		

<p>Description (continued)</p>	<p>Where in nican.h:</p> <pre>#define NC_FL_CAN_ARBID_INFO 0x40000000 #define NC_ARBID_INFO_RTSM_INPUT 0x00000001</pre> <p>IsRemote: Unchanged</p> <p>DataLength: RTSM line number that produces the event</p> <p>Data[8]: Unchanged</p> <p>NC_RTSM_OUT_ON_RX (RTSM Output on Receiving CAN Frame):</p> <p>In this mode, NI-CAN will output an RTSM trigger on the line configured via NC_ATTR_RTSM_SIGNAL (RTSM Line Number) whenever a frame is enqueued in the read queue of that object.</p> <p>NC_RTSM_OUT_ON_TX (RTSM Output on Transmitting CAN Frame):</p> <p>In this mode, NI-CAN will output an RTSM trigger on the line configured via NC_ATTR_RTSM_SIGNAL (RTSM Line Number) whenever a frame is successfully transmitted.</p> <p>NC_RTSM_OUT_ACTION_ONLY (RTSM Output on ncAction call):</p> <p>In this mode, NI-CAN will output an RTSM trigger on the line configured via NC_ATTR_RTSM_SIGNAL whenever the user calls the ncAction function. With this function, a user can set/toggle an RTSM line high or low.</p>
-------------------------------------------	------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

NC_ATTR_RTSM_SIGNAL (RTSM Line Number)

Attribute Id	NC_ATTR_RTSM_SIGNAL (RTSM Line Number)
Hex Encoding	0x80000018
Data Type	NCTYPE_UINT32
Permissions	Config, Set, Get
Description	<p>This attribute defines the RTSM B signal to be associated with the CAN object.</p> <p>Attribute values: 0 to 7 (for RTSM B signal lines)</p> <p>Note: In the hardware, four RTSM lines are for input and four lines are for output. Hence, four CAN objects can configure RTSM lines as input and four can configure RTSM lines as output. An error 0x8000000D (#define NC_ERR_RSRC_LIMITS 0x0000000D) will be reported when these limits are exceeded.</p> <p>Note: For low-speed and dual-speed boards, two lines are available as input and three (3) lines are available as output. The unavailable lines are used for low-speed transceiver fault reporting.</p> <p>There is no limitation on which lines can be used as input or output.</p>

NC_ATTR_RTSM_SIG_BEHAV (RTSM Behavior)

Attribute Id	NC_ATTR_RTSM_SIG_BEHAV (RTSM Behavior)
Hex Encoding	0x80000019
Data Type	NCTYPE_UINT32
Permissions	Config, Set, Get
Description	<p>This attribute is used when a CAN object is used to output RTSM signals and defines whether the RTSM line is pulsed or toggled.</p> <p>Attribute values:</p> <p>NC_RTSM_SIG_PULSE (Output RTSM Pulse): This pulses the RTSM line with a 100 μs pulse.</p> <p>NC_RTSM_SIG_TOGGLE (Toggle RTSM Line): This toggles the RTSM line. If the previous state was high, it will be toggled low, and vice versa.</p>

NC_ATTR_RTISI_SKIP (RTISI Skip)

Attribute Id	NC_ATTR_RTISI_SKIP (RTISI Skip)
Hex Encoding	0x80000021
Data Type	NCTYPE_UINT32
Permissions	Config, Set, Get
Description	<p>This attribute defines the number of RTISI events to skip before logging them to the read queue for that object. This attribute is used with NC_ATTR_RTISI_MODE and with an attribute value of NC_RTISI_TIME_ON_IN.</p> <p>Attribute values: Any user number.</p>

CAN Object

Object Name

CANx::STD*Arbitration ID*

CANx::XTD*Arbitration ID*

CANx is the name of a CAN Network Interface Object such as CAN0. The letters STD and XTD indicate the class of the CAN Object, specifying whether it uses a standard (11-bit) arbitration ID or an extended (29-bit) arbitration ID. You normally specify the actual *Arbitration ID* of the CAN Object as a decimal number, but you can use hexadecimal notation by including a “0x” at the beginning of the hexadecimal notation.

Encapsulates

CAN arbitration ID and its associated data.

Description

When a network frame is transmitted on a CAN-based network, it always begins with the arbitration ID. This arbitration ID is primarily used for collision resolution when more than one frame is transmitted simultaneously, but often is also used as a simple mechanism to identify data. The CAN arbitration ID, along with its associated data, is referred to as a CAN Object.

The NI-CAN implementation of CAN provides high-level access to CAN Objects on an individual basis. You can configure each CAN Object for different forms of communication (such as periodic polling, receiving unsolicited CAN data frames, and so on). After you configure a CAN Object and open it for communication, use the `ncRead` and `ncWrite`

functions to access the data of the CAN Object. The NI-CAN driver performs all other details regarding the object.

Attributes

NC_ATTR_CAN_DATA_LENGTH (Data Length)

Attribute ID	NC_ATTR_CAN_DATA_LENGTH
Hex Encoding	80010007
Data Type	NCTYPE_UINT32
Permissions	Config
Description	NC_ATTR_CAN_DATA_LENGTH indicates the number of bytes of data contained in CAN data frames for the CAN Object. This number is also placed into the Data Length Code (DLC) field of transmitted CAN data frames or CAN remote frames (although CAN remote frames do not contain actual data bytes).

NC_ATTR_CAN_TX_RESPONSE (Transmit by Response)

Attribute ID	NC_ATTR_CAN_TX_RESPONSE
Hex Encoding	80010006
Data Type	NCTYPE_BOOL
Permissions	Config
Description	<p>The NC_ATTR_CAN_TX_RESPONSE attribute applies only to CAN Object configurations in which the Communication Type (NC_ATTR_COMM_TYPE) is set to Transmit Data by Call, Transmit Data Periodically, or Transmit Periodic Waveform. For those configurations, NC_ATTR_CAN_TX_RESPONSE specifies whether the CAN Object should automatically respond with the previously transmitted CAN data frame when it detects an incoming CAN remote frame. When set to NC_FALSE, the CAN Object transmits CAN data frames only as configured, and ignores all incoming CAN remote frames for its arbitration ID. When set to NC_TRUE, the CAN Object responds to incoming CAN remote frames. CAN data frames transmitted due to incoming CAN remote frames are independent of any CAN data frames transmitted as a result of configured behavior.</p> <p>If you know that a given CAN Object will not receive CAN remote frames, you should set this attribute to NC_FALSE so that NI-CAN can ignore such frames.</p>

NC_ATTR_COMM_TYPE (Communication Type)

Attribute ID	NC_ATTR_COMM_TYPE
Hex Encoding	80000016
Data Type	NCTYPE_UINT32
Permissions	Config
Description	The NC_ATTR_COMM_TYPE (Communication Type) attribute configures the fundamental behavior of the CAN Object. The values for Communication Type are described in the Values for Communication Type section, later in this chapter. Values that Receive are always used to receive CAN data frames (and possibly transmit CAN remote frames). Values that Transmit are always used to transmit CAN data frames (and possibly receive CAN remote frames).

NC_ATTR_PERIOD (Period)

Attribute ID	NC_ATTR_PERIOD
Hex Encoding	8000000F
Data Type	NCTYPE_DURATION
Permissions	Config
Description	<p>When you set the Communication Type (NC_ATTR_COMM_TYPE) to Transmit Data Periodically, Transmit Periodic Waveform, or Receive Periodically Using Remote, this attribute specifies the time in milliseconds between subsequent transmissions.</p> <p>When you set the Communication Type to Receive Unsolicited or Transmit by Response Only, this attribute specifies a watchdog timeout. A watchdog timeout of zero disables the watchdog timer.</p> <p>When you set the Communication Type to Transmit Data by Call or Receive Data By Call Using Remote, this attribute specifies the minimum interval between subsequent transmissions. A minimum interval of zero disables the minimum interval timer.</p>

NC_ATTR_READ_PENDING (Read Entries Pending)

Attribute ID	NC_ATTR_READ_PENDING
Hex Encoding	80000011
Data Type	NCTYPE_UINT32
Permissions	Get
Description	Indicates the number of pending entries in the read queue. If NC_ATTR_READ_PENDING is zero, the NC_ST_READ_AVAIL state is clear.

NC_ATTR_READ_Q_LEN (Read Queue Length)

Attribute ID	NC_ATTR_READ_Q_LEN
Hex Encoding	80000013
Data Type	NCTYPE_UINT32
Permissions	Config
Description	Length (maximum number of entries) for the read queue. For more information, refer to the description of the ncRead function in Chapter 2, <i>NI-CAN Functions</i> .

NC_ATTR_READ_MULT_SIZE

Attribute Id	NC_ATTR_READ_MULT_SIZE
Hex Encoding	0x8001000B
Data Type	NCTYPE_UINT32
Permissions	Config, Set, Get
Description	<p>Sets the size (in number of frames) that NI-CAN will use to notify the user when specified amount of frames are available in the Read Queue. Once the application receives the notification, the user can call <code>ncReadMult</code> to read the desired number of frames. By using this functionality, a user does not need to poll the queue constantly to read frames.</p> <p>Note that the <code>ncCreateNotification</code> (or <code>ncCreateOccurrence</code>) function must use a desired state of <code>NC_ST_READ_MULT</code> (hex encoding <code>0x00000008</code>).</p> <p>In LabVIEW, the attribute can be set by using the <code>ncSetAttribute</code> function after calling <code>ncConfig</code> and <code>ncOpen</code> for the object. The user then needs to call <code>ncCreateOccurrence</code>, as shown in this manual, with the aforementioned state (<code>0x08</code>) as the Desired State.</p> <p>In C, you can do this by either adding it to the Network Interface attribute configuration or calling the <code>ncSetAttribute</code> function. The function call to <code>ncCreateNotification</code> must have the Desired State of <code>NC_ST_READ_MULT</code>.</p>

NC_ATTR_RTSI_MODE (RTSI Mode)

Attribute Id	NC_ATTR_RTSI_MODE
Hex Encoding	0x80000017
Data Type	NCTYPE_UINT32
Permissions	Config, Set, Get

Description	<p>This attribute defines whether the user needs to configure the CAN object as an RTSI driver or the DAQ board as the RTSI driver. The following values can be used:</p> <p>Attribute values:</p> <table border="0"> <tr> <td>In C</td> <td>In LabVIEW RTSI Config Cluster</td> </tr> <tr> <td>NC_RTSI_NONE</td> <td>Disable RTSI</td> </tr> <tr> <td>NC_RTSI_TX_ON_IN</td> <td>On RTSI Input—Transmit CAN Frame</td> </tr> <tr> <td>NC_RTSI_TIME_ON_IN</td> <td>On RTSI Input—Timestamp RTSI event</td> </tr> <tr> <td>NC_RTSI_OUT_ON_RX</td> <td>RTSI Output on Receiving CAN Frame</td> </tr> <tr> <td>NC_RTSI_OUT_ON_TX</td> <td>RTSI Output on Transmitting CAN Frame</td> </tr> <tr> <td>NC_RTSI_OUT_ACTION_ONLY</td> <td>RTSI Output on ncAction call</td> </tr> </table> <p>Each of the mode is explained in detail below.</p> <p>NC_RTSI_TX_ON_IN (On RTSI Input-Transmit CAN Frame):</p> <p>In this mode, NI-CAN will transmit the most recent frame on an incoming RTSI trigger on the RTSI line configured via NC_ATTR_RTSI_SIGNAL. The CAN Object can be configured as:</p> <ul style="list-style-type: none"> • NC_CAN_COMM_TX_BY_CALL (transmit frame by calling ncWrite) • NC_CAN_COMM_TX_PERIODIC (periodic transmission) • NC_CAN_COMM_TX_WAVEFORM (waveform transmit) <p>In all three configurations, a CAN frame is transmitted on every incoming RTSI trigger. The period is ignored (if nonzero). (Note: for transmitting waveform, follow the instructions in the CAN Object section.)</p>	In C	In LabVIEW RTSI Config Cluster	NC_RTSI_NONE	Disable RTSI	NC_RTSI_TX_ON_IN	On RTSI Input—Transmit CAN Frame	NC_RTSI_TIME_ON_IN	On RTSI Input—Timestamp RTSI event	NC_RTSI_OUT_ON_RX	RTSI Output on Receiving CAN Frame	NC_RTSI_OUT_ON_TX	RTSI Output on Transmitting CAN Frame	NC_RTSI_OUT_ACTION_ONLY	RTSI Output on ncAction call
In C	In LabVIEW RTSI Config Cluster														
NC_RTSI_NONE	Disable RTSI														
NC_RTSI_TX_ON_IN	On RTSI Input—Transmit CAN Frame														
NC_RTSI_TIME_ON_IN	On RTSI Input—Timestamp RTSI event														
NC_RTSI_OUT_ON_RX	RTSI Output on Receiving CAN Frame														
NC_RTSI_OUT_ON_TX	RTSI Output on Transmitting CAN Frame														
NC_RTSI_OUT_ACTION_ONLY	RTSI Output on ncAction call														

<p>Description (continued)</p>	<p>For an object configured with <code>NC_CAN_COMM_TX_BY_CALL</code>, transmission is begun by writing a frame containing the write queue of the object (by calling <code>ncWrite</code>) and an RTSI signal applied to the configured RTSI line. NI-CAN will retransmit the last frame until a new frame is enqueued.</p> <p>NC_RTSI_TIME_ON_IN (On RTSI Input—Timestamp RTSI event):</p> <p>In this mode, NI-CAN will timestamp an incoming RTSI trigger on the RTSI line configured via <code>NC_ATTR_RTSI_SIGNAL</code> and enqueue (in the object's read queue) a frame containing special entries in the following fields (as noted):</p> <p>Timestamp: Time when RTSI event occurred.</p> <p>Data[8]: User-defined frame (first 4 bytes) defined by <code>NC_ATTR_RTSI_FRAME</code>. See description of the <code>NC_ATTR_RTSI_FRAME</code> attribute for more details.</p> <p>NC_RTSI_OUT_ON_RX (RTSI Output on Receiving CAN Frame):</p> <p>In this mode, NI-CAN will output an RTSI trigger on the line configured via <code>NC_ATTR_RTSI_SIGNAL</code> (RTSI Line Number) whenever a frame is enqueued in that object's read queue. This RTSI configuration can be used when the Object is configured as:</p> <p><code>NC_CAN_COMM_RX_UNSOL</code> (Receive Unsolicited)</p> <p>NC_RTSI_OUT_ON_TX (RTSI Output on Transmitting CAN Frame):</p> <p>In this mode, NI-CAN will output an RTSI trigger on the line configured via <code>NC_ATTR_RTSI_SIGNAL</code> (RTSI Line Number) whenever a frame is successfully transmitted. You can use this RTSI configuration when the object is configured as:</p> <ul style="list-style-type: none"> • <code>NC_CAN_COMM_TX_BY_CALL</code> (Transmit Data by call) • <code>NC_CAN_COMM_TX_PERIODIC</code> (Transmit Data Periodically) • <code>NC_CAN_COMM_TX_WAVEFORM</code> (Transmit Periodic Waveform) <p>NC_RTSI_OUT_ACTION_ONLY (RTSI Output on ncAction call):</p> <p>In this mode, NI-CAN will output an RTSI trigger on the line configured via <code>NC_ATTR_RTSI_SIGNAL</code> whenever the user calls the <code>ncAction</code> function. With this function, a user can set/toggle an RTSI line high or low.</p>
---------------------------------------	---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

NC_ATTR_RTISI_SIGNAL (RTSI Line Number)

Attribute Id	NC_ATTR_RTISI_SIGNAL (RTSI Line Number)
Hex Encoding	0x80000018
Data Type	NCTYPE_UINT32
Permissions	Config, Set, Get
Description	<p>This attribute defines the RTSI B signal to be associated with the CAN object.</p> <p>Attribute values: 0 to 7 (for RTSI B signal lines).</p> <p>Note: In the hardware, four RTSI lines are for input and four lines are for output. Hence, four CAN objects can configure RTSI lines for input and four CAN objects can configure RTSI lines for output. An error 0x8000000D (#define NC_ERR_RSRC_LIMITS 0x0000000D) will be reported when these limits are exceeded.</p> <p>Note: For low-speed and dual-speed boards, two lines are available as inputs and three (3) lines are available as outputs. The unavailable lines are used for low-speed transceiver fault reporting.</p> <p>There is no limitation on which lines can be used as input or output.</p>

NC_ATTR_RTISI_SIG_BEHAV (RTSI Behavior)

Attribute Id	NC_ATTR_RTISI_SIG_BEHAV (RTSI Behavior)
Hex Encoding	0x80000019
Data Type	NCTYPE_UINT32
Permissions	Config, Set, Get
Description	<p>This attribute is to be used when a CAN object is used to output RTSI signals and defines if the RTSI line is to be pulsed or toggled.</p> <p>Attribute values:</p> <p>NC_RTISISIG_PULSE (Output RTSI Pulse): This pulses the RTSI line with a 100 μs pulse.</p> <p>NC_RTISISIG_TOGGLE (Toggle RTSI Line): This toggles the RTSI line. If the previous state was high, it will be toggled low, and vice versa.</p>

NC_ATTR_RTISI_FRAME (User RTISI Frame)

Attribute Id	NC_ATTR_RTISI_FRAME (UserRtsiFrame)
Hex Encoding	0x80000020
Data Type	NCTYPE_UINT32
Permissions	Config, Set, Get
Description	<p>Use this attribute when a CAN object is to be configured with the attribute NC_ATTR_RTISI_MODE and an attribute value of NC_RTISI_TIME_ON_IN.</p> <p>Because the CAN object's receiving structure contains only the Timestamp and Data[8] fields, you must specify a 4-byte data frame that NI-CAN can use in the first four bytes of the Data[8] field, to help distinguish the RTISI event from other data frames. This user frame is configured via the NC_ATTR_RTISI_FRAME attribute in the RTISI configuration for the CAN object.</p> <p>Attribute values: Any user-defined unsigned32 number in hex. For example, 0xAABBCCDD.</p> <p>Note: In LabVIEW the default configuration is 0x5254349 which is the ASCII value for RTISI.</p>

NC_ATTR_RTISI_SKIP (RTISI Skip)

Attribute Id	NC_ATTR_RTISI_SKIP (RTISI Skip)
Hex Encoding	0x80000021
Data Type	NCTYPE_UINT32
Permissions	Config, Set, Get
Description	<p>This attribute defines the number of RTISI events to skip before logging them to the read queue for that object. Use this attribute with NC_ATTR_RTISI_MODE and with an attribute value of NC_RTISI_TIME_ON_IN.</p> <p>Attribute values: Any user number.</p>

NC_ATTR_RX_CHANGES_ONLY (Receive Changes Only)

Attribute ID	NC_ATTR_RX_CHANGES_ONLY
Hex Encoding	80000015
Data Type	NCTYPE_BOOL
Permissions	Config
Description	<p>The NC_ATTR_RX_CHANGES_ONLY attribute applies only to CAN Object configurations in which the Communication Type (NC_ATTR_COMM_TYPE) is set to Receive CAN data frames. For those configurations, if NC_ATTR_RX_CHANGES_ONLY is set to NC_FALSE, NI-CAN places data from all incoming CAN data frames into the read queue. If this attribute is set to NC_TRUE, NI-CAN places data from an incoming CAN data frame into the read queue only if it differs from the previously received data.</p> <p>This attribute has no effect on the usage of a watchdog timeout for the CAN Object. For example, if this attribute is true and you also specify a watchdog timeout, NI-CAN restarts the watchdog timeout every time it receives a CAN data frame from the network, regardless of whether the data differs from the previous value.</p>

NC_ATTR_STATE (Object State)

Attribute ID	NC_ATTR_STATE
Hex Encoding	80000009
Data Type	NCTYPE_STATE
Permissions	Get
Description	Current state of the CAN Object. In most cases, the NC_ST_STOPPED, NC_ST_WARNING, and NC_ST_ERROR states are merely reflected up from the underlying CAN Network Interface Object.

NC_ATTR_STATUS (Object Status)

Attribute ID	NC_ATTR_STATUS
Hex Encoding	8000000A
Data Type	NCTYPE_STATUS
Permissions	Get
Description	Background status of the CAN Object. Unless the NC_ST_WARNING or NC_ST_ERROR states are set in NC_ATTR_STATE, this attribute is always NC_SUCCESS. When you read an error or warning from this attribute, NI-CAN clears the appropriate state, and the background status is set back to NC_SUCCESS. For communication errors such as NC_ERR_CAN_BUS_OFF, this background status is the same as the background status of the underlying CAN Network Interface Object. If a background error occurs, you can read it from this attribute, or obtain it from the next call to ncRead or ncWrite.

NC_ATTR_WRITE_PENDING (Write Entries Pending)

Attribute ID	NC_ATTR_WRITE_PENDING
Hex Encoding	80000012
Data Type	NCTYPE_UINT32
Permissions	Get
Description	Indicates the number of pending entries in the write queue. If NC_ST_WRITE_PENDING is zero, the NC_ST_WRITE_SUCCESS state is set (after NI-CAN successfully transmits the final frame).

NC_ATTR_WRITE_Q_LEN (Write Queue Length)

Attribute ID	NC_ATTR_WRITE_Q_LEN
Hex Encoding	80000014
Data Type	NCTYPE_UINT32
Permissions	Config
Description	Length (maximum number of entries) for the write queue. For more information, refer to the description of the ncWrite function in Chapter 2, <i>NI-CAN Functions</i> .

Values for Communication Type

The following sections describe the allowable values for `NC_ATTR_COMM_TYPE` (Communication Type).

Receive Unsolicited (NC_CAN_COMM_RX_UN SOL)

Use this configuration to receive unsolicited CAN data frames from a remote device.

If the CAN data frames are expected periodically, you can use a watchdog timeout by setting `Period` (`NC_ATTR_PERIOD`) to the desired number of milliseconds. Then, when the CAN Object detects an incoming CAN data frame, it restarts the watchdog timeout. If the watchdog timeout expires before the next incoming CAN data frame is received for the CAN Object, NI-CAN reports a `NC_ERR_TIMEOUT` error. The watchdog timeout is used to verify that the remote node still exists and is transmitting data as expected. If you do not want to use a watchdog timeout, set `Period` to zero.

The `Receive Changes Only` (`NC_ATTR_RX_CHANGES_ONLY`) attribute can be used to receive all data (`NC_FALSE`) or only changes (`NC_TRUE`).

Because this CAN Object does not transmit CAN data frames, the `Transmit by Response` (`NC_ATTR_CAN_TX_RESPONSE`) attribute is ignored (assumes `NC_FALSE`).

RTSI: This Object configuration supports two RTSI modes:

- `NC_RTSTIME_ON_IN` (On RTSI Input—Timestamp RTSI event)
- `NC_RTSTIME_OUT_ON_RX` (RTSI Output on Receiving CAN Frame)

Refer to the *CAN Object* attributes section for information on using these RTSI attributes.

Receive Periodically Using Remote (NC_CAN_COMM_RX_PERIODIC)

Use this configuration to poll for data from a remote device periodically. Every period, the object transmits a CAN remote frame, and NI-CAN places the resulting CAN data frame response into the read queue.

The `Period` (`NC_ATTR_PERIOD`) attribute is used to configure the period between successive CAN remote frame transmissions.

The `Receive Changes Only` (`NC_ATTR_RX_CHANGES_ONLY`) attribute can be used to receive all data (`NC_FALSE`), or only changes (`NC_TRUE`).

Because this CAN Object does not transmit CAN data frames, the `Transmit by Response` (`NC_ATTR_CAN_TX_RESPONSE`) attribute is ignored (assumes `NC_FALSE`).

Receive Value by Call Using Remote (NC_CAN_COMM_RX_BY_CALL)

Use this configuration to poll for data from a remote device using the `ncWrite` function. You must call `ncWrite` with `DataSize` zero to transmit a CAN remote frame. NI-CAN places the resulting CAN data frame response into the read queue.

If you want to specify the minimum amount of time between subsequent transmission of CAN remote frames, you can specify a minimum interval by setting `Period (NC_ATTR_PERIOD)` to the desired number of milliseconds. You configure the minimum interval as a promise to other nodes on the network that the object will not transmit its CAN frames with needless frequency, thus precluding transfer by lower priority CAN frames. You can use a write queue in conjunction with the minimum intervals to guarantee that the desired number of frames is transmitted on the network.

The Receive Changes Only (`NC_ATTR_RX_CHANGES_ONLY`) can be used to receive all data (`NC_FALSE`) or only changes (`NC_TRUE`).

Because this CAN Object does not transmit CAN data frames, the Transmit by Response (`NC_ATTR_CAN_TX_RESPONSE`) attribute is ignored (assumes `NC_FALSE`).

Transmit Data Periodically (NC_CAN_COMM_TX_PERIODIC)

Use this configuration to transmit a CAN data frame to a remote device periodically. The `Period (NC_ATTR_PERIOD)` attribute is used to configure the period between successive CAN data frame transmissions.

When NI-CAN transmits the last entry of the write queue, that entry is used every period until you provide a new entry using `ncWrite`. With this behavior, every entry is guaranteed to be transmitted at least once, and the object always has data available for transmission. If the write queue is empty when communication starts, the first periodic transmission does not occur until you provide a valid data value using `ncWrite`.

Because this CAN Object does not receive CAN data frames, the Receive Changes Only (`NC_ATTR_RX_CHANGES_ONLY`) attribute is ignored (assumes `NC_FALSE`).

The Transmit by Response (`NC_ATTR_CAN_TX_RESPONSE`) attribute can be used to ignore incoming CAN remote frames (`NC_FALSE`), or to transmit previous data when a CAN remote frame is received (`NC_TRUE`).

RTSI: This Object configuration supports two RTSI modes:

- `NC_RTSI_TX_ON_IN` (On RTSI Input—Transmit CAN Frame)
- `NC_RTSI_OUT_ON_TX` (RTSI Output on Transmitting CAN Frame)

Refer to the *CAN Object* attributes section for information on using these RTSI attributes.

Transmit Value by Response Only (NC_CAN_COMM_TX_RESP_ONLY)

Use this configuration to transmit CAN data frames only in response to an incoming CAN remote frame. When you call `ncWrite`, the data is placed in the write queue, and remains there until a CAN remote frame is received.

If the CAN remote frames are expected periodically, you can specify a watchdog timeout by setting `Period (NC_ATTR_PERIOD)` to the desired number of milliseconds. Then, when the CAN Object detects an incoming CAN remote frame, it restarts the watchdog timeout. If the watchdog timeout expires before the next incoming CAN remote frame is received for the CAN Object, NI-CAN reports an `NC_ERR_TIMEOUT` error. The watchdog timeout is used to verify that the remote node still exists and is transmitting CAN remote frames as expected. If you do not want to use a watchdog timeout, set `Period` to zero.

Because this CAN Object does not receive CAN data frames, the `Receive Changes Only (NC_ATTR_RX_CHANGES_ONLY)` attribute is ignored (assumes `NC_FALSE`).

Because this CAN Object always responds to incoming CAN remote frames, the `Transmit by Response (NC_ATTR_CAN_TX_RESPONSE)` attribute is ignored (assumes `NC_TRUE`).

Transmit Data by Call (NC_CAN_COMM_TX_BY_CALL)

Use this configuration to transmit a CAN data frame when `ncWrite` is called.

If you want to specify the minimum amount of time between subsequent transmission of CAN data frames, you can specify a minimum interval by setting `Period (NC_ATTR_PERIOD)` to the desired number of milliseconds (see *Receive Value by Call Using Remote*, earlier in this chapter).

Because this CAN Object does not receive CAN data frames, the `Receive Changes Only (NC_ATTR_RX_CHANGES_ONLY)` attribute is ignored (assumes `NC_FALSE`).

The `Transmit by Response (NC_ATTR_CAN_TX_RESPONSE)` attribute can be used to ignore incoming CAN remote frames (`NC_FALSE`), or to transmit previous data when a CAN remote frame is received (`NC_TRUE`).

RTSI: This Object configuration supports two RTSI modes:

- `NC_RTSI_TX_ON_IN` (On RTSI Input—Transmit CAN Frame)
- `NC_RTSI_OUT_ON_TX` (RTSI Output on Transmitting CAN Frame)

Refer to the *CAN Object* attributes section for information on using these RTSI attributes.

Transmit Periodic Waveform (NC_CAN_COMM_TX_WAVEFORM)

Use this configuration to transmit a fixed sequence of CAN data frames over and over, one CAN data frame every period. By varying the data value in each CAN data frame, this configuration can be used to transmit a waveform to a remote device.

The Period (NC_ATTR_PERIOD) attribute is used to configure the period between successive CAN data frame transmissions.

Because this CAN Object does not receive CAN data frames, the Receive Changes Only (NC_ATTR_RX_CHANGES_ONLY) attribute is ignored (assumes NC_FALSE).

The Transmit by Response (NC_ATTR_CAN_TX_RESPONSE) attribute can be used to ignore incoming CAN remote frames (NC_FALSE), or to transmit previous data when a CAN remote frame is received (NC_TRUE).

The following steps illustrate the typical usage of Transmit Periodic Waveform.

1. Configure the CAN Network Interface Object with Start On Open false, then configure the object.
2. Configure the CAN Object as Transmit Periodic Waveform and set a nonzero Write Queue length, then open the Object.
3. Call `ncWrite` for the CAN Object, once for every entry specified for the Write Queue Length.
4. Use `ncAction` to start the CAN Network Interface Object (not the CAN Object).
The CAN Object transmits the first entry in the write queue, then waits the specified Period, then transmits the second entry, and so on. After the last entry is transmitted, the CAN Object waits the specified Period, then transmits the first entry again.
5. You can use `ncAction` to stop and restart the CAN Object's transmissions. When the CAN Object is stopped, you can use `ncWrite` to provide new waveform entries. When the write queue is full, `ncWrite` always replaces the first (oldest) entry in the queue.

RTSI: This Object configuration supports two RTSI modes:

- NC_RTSI_TX_ON_IN (On RTSI Input—Transmit CAN Frame)
- NC_RTSI_OUT_ON_TX (RTSI Output on Transmitting CAN Frame)

Refer to the [CAN Object](#) attributes section for information on using these RTSI attributes.

Examples of Different Communication Types

The following figures demonstrate how you can use the Communication Type attribute for actual network data transfer. Each figure shows two separate NI-CAN applications that are physically connected across a CAN network.

Figure 3-1 shows a CAN Object that periodically transmits data to another CAN Object. The receiving CAN Object can queue up to five data values.

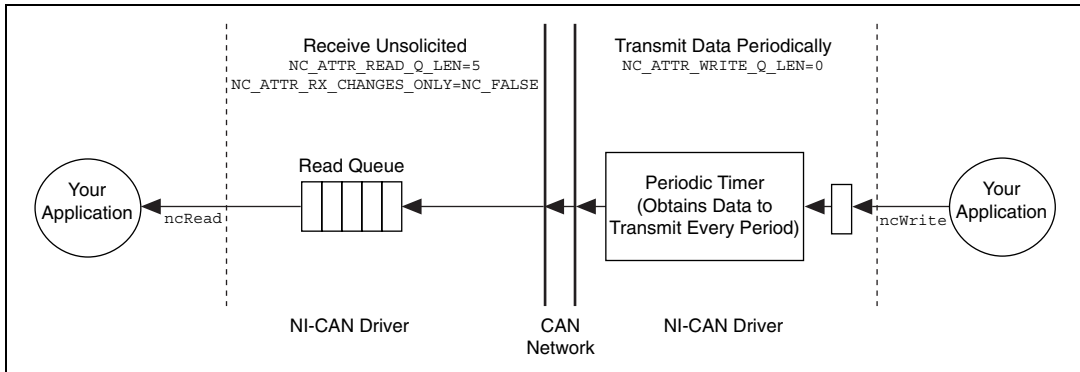


Figure 3-1. Example of Periodic Transmission

Figure 3-2 shows a CAN Object that polls data from another CAN Object. NI-CAN transmits the CAN remote frame when you call `ncWrite`.

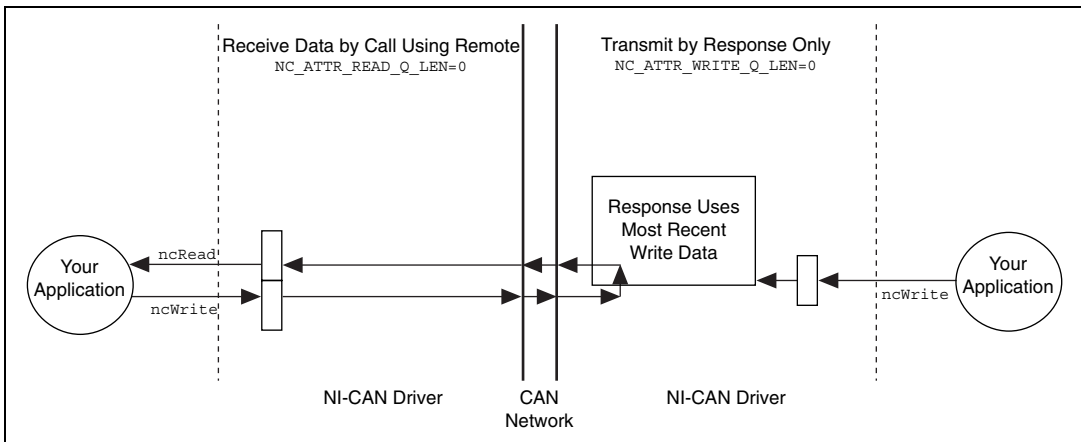


Figure 3-2. Example of Polling Remote Data Using `ncWrite`

Figure 3-3 shows a CAN Object that polls data from another CAN Object. NI-CAN transmits the remote frame periodically and places only changed data into the read queue.

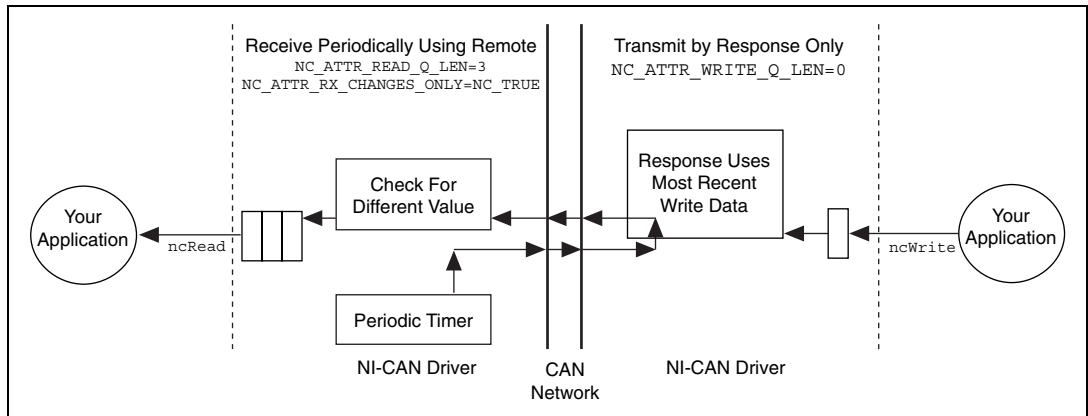


Figure 3-3. Example of Periodic Polling of Remote Data

RTSI Programming

This chapter consolidates the Real Time System Integration (RTSI) programming features available in NI-CAN. This information is also in the [CAN Network Interface Object](#) and [CAN Object](#) attributes sections of Chapter 3, [NI-CAN Objects](#), and is useful when used in conjunction with the object specifics.

Description

RTSI is a bus that interconnects National Instruments DAQ, IMAQ, Motion, and CAN boards. This feature allows synchronization of DAQ, IMAQ, Motion, and CAN boards by allowing exchange of timing signals. Using RTSI, a device (board) can control one or more slave devices. PCI/AT boards require a ribbon cable for the connections, but for PXI boards the connections are available on the PXI chassis backplane. Refer to the getting started manual for your version of the Windows operating system for more details on the hardware connector.

In NI-CAN, RTSI is configured via attributes in either the Network Interface or the CAN Object configuration.

In C, the configuration is done by adding new elements to `AttributeIdList` and `AttrValueList` before calling `ncConfig`.

In LabVIEW, the configuration is done via the Network Interface Config cluster or the CAN Object Configuration Cluster, which has an optional input to wire an RTSI configuration cluster. Refer to the `ncConfig` function for further details.

The following is a summary of the attributes and possible values that these attributes can have. For hex encoding of the attributes, refer to the [CAN Network Interface Object](#) or [CAN Object](#) attributes sections of Chapter 3, [NI-CAN Objects](#), or to the `nican.h` file.

Attributes

NC_ATTR_RTISI_MODE (RTSI Mode)

This attribute defines whether a CAN object is to be configured as a RTSI slave or master. The following values can be used:

Attribute Values in C	Attribute Values in LabVIEW
NC_RTISI_NONE	Disable RTSI
NC_RTISI_TX_ON_IN	On RTSI Input—Transmit CAN Frame
NC_RTISI_TIME_ON_IN	On RTSI Input—Timestamp RTSI event
NC_RTISI_OUT_ON_RX	RTSI Output on Receiving CAN Frame
NC_RTISI_OUT_ON_TX	RTSI Output on Transmitting CAN Frame
NC_RTISI_OUT_ACTION_ONLY	RTSI Output on <code>ncAction</code> call

The attribute values are described below.

NC_RTISI_NONE (Disable RTSI)

No RTSI use is needed for this object. If the object is set to this value, all other RTSI configuration is ignored.

NC_RTISI_TX_ON_IN (On RTSI Input—Transmit CAN Frame)

Network Interface: In this mode, NI-CAN will transmit the most recent frame on an incoming RTSI trigger on the RTSI line configured via `NC_ATTR_RTISI_SIGNAL`. To begin transmission, a frame must be written to the write queue of the object (by calling `ncWrite`) and an RTSI signal applied to the configured RTSI line. NI-CAN will retransmit the last frame until a new frame is enqueued.

CAN Object: In this mode, the CAN Object can be configured as:

- `NC_CAN_COMM_TX_BY_CALL` (transmit frame by calling `ncWrite`)
- `NC_CAN_COMM_TX_PERIODIC` (periodic transmission)
- `NC_CAN_COMM_TX_WAVEFORM` (waveform transmit)

In all of the three configurations, a CAN frame is transmitted on every incoming RTSI trigger. The period is ignored (if nonzero). Refer to the *CAN Object* section of Chapter 3, *NI-CAN Objects*, for instructions to set up the CAN object for each communication type.

NC_RTSI_TIME_ON_IN (On RTSI Input—Timestamp RTSI event)

Network Interface: In this mode, NI-CAN will timestamp an incoming RTSI trigger on the RTSI line configured via `NC_ATTR_RTSI_SIGNAL` and enqueue (in the object's read queue) a frame containing special entries in the following fields (as noted):

Timestamp: Time when RTSI event occurred

ArbitrationId: `0x40000001`
`(NC_FL_CAN_ARBITD_INFO |`
`NC_ARBITD_INFO_RTSI_INPUT)`

Hex coding:

`NC_FL_CAN_ARBITD_INFO` `0x40000000`

`NC_ARBITD_INFO_RTSI_INPUT` `0x00000001`

IsRemote: unchanged

DataLength: RTSI line number that produces the event

Data[8]: unchanged

CAN Object: Because the CAN object's receiving structure contains only the `Timestamp` and `Data[8]` fields, you must specify a 4-byte data frame that NI-CAN can use in the first four bytes of the `Data[8]` field, to help distinguish the RTSI event from other data frames. This user frame is configured via the `NC_ATTR_RTSI_FRAME` attribute in the CAN object RTSI configuration.

This attribute is ignored when a Network Interface is being configured.

NC_RTSI_OUT_ON_RX (RTSI Output on Receiving CAN frame)

Network Interface & CAN Objects: In this mode, NI-CAN will output an RTSI trigger on the line configured via `NC_ATTR_RTSI_SIGNAL` whenever a frame is enqueued in the object read queue.

NC_RTISI_OUT_ON_TX (RTSI Output on Transmitting CAN frame)

Network Interface & CAN Objects: In this mode, NI-CAN will output an RTSI trigger on the line configured via `NC_ATTR_RTISI_SIGNAL` whenever a frame is successfully transmitted.

NC_RTISI_OUT_ACTION_ONLY (RTSI Output on ncAction call)

Network Interface & CAN Objects: In this mode, NI-CAN will output an RTSI trigger on the line configured via `NC_ATTR_RTISI_SIGNAL` whenever user calls the `ncAction` function. With this function, a user can set/toggle a RTSI line high or low.

NC_ATTR_RTISI_SIGNAL (RTSI Line Number)

This attribute defines the RTSI signal that must be associated with the CAN object. This attribute must be used with the Network Interface and CAN objects for all desired RTSI modes.

Attribute values: 0 to 7 (for RTSI signal lines).



Note In the hardware, four RTSI lines are for input and four lines are for output. Hence, four CAN objects can configure RTSI lines for input and four CAN objects can configure RTSI lines for output. An error `0x8000000D` (`#define NC_ERR_RSRC_LIMITS 0x0000000D`) will be reported when these limits are exceeded.



Note For low-speed and dual-speed boards, two lines are available as inputs and three (3) lines are available as outputs. The unavailable lines are used for low-speed transceiver fault reporting.

There is no limitation on which RTSI line number can be used as input or output.

NC_ATTR_RTISI_SIG_BEHAV (RTSI Behavior)

Use this attribute when a CAN object is used to output RTSI signals when CAN is the RTSI driver. This attribute must be used with the Network Interface and CAN objects that output an RTSI trigger.

Attribute Values in C	Attribute Values in LabVIEW
<code>NC_RTISISIG_PULSE</code>	Output RTSI Pulse
<code>NC_RTISISIG_TOGGLE</code>	Toggle RTSI Line

The attribute values are:

- `NC_RTSSIG_PULSE` (Output RTSI Pulse): This pulses the RTSI line with a 100 μ s pulse.
- `NC_RTSSIG_TOGGLE` (Toggle RTSI Line): This toggles the RTSI line. If the previous state was high, it will be toggled low, and vice versa.

NC_ATTR_RTSSI_FRAME (UserRTSIFrame)

Use this attribute when a CAN object is to be configured with the attribute `NC_ATTR_RTSSI_MODE` and with an attribute value of `NC_RTSSI_TIME_ON_IN`.

Because the CAN object's receiving structure contains only the Timestamp and Data[8] fields, you must specify a 4-byte data frame that NI-CAN can use in the first four bytes of the Data[8] field, to help distinguish the RTSI event from other data frames. This user frame is configured via the `NC_ATTR_RTSSI_FRAME` attribute in the RTSI configuration for the CAN object.

Attribute values: Any user-defined unsigned32 number in hex. For example, `0xAABBCCDD`.

NC_ATTR_RTSSI_SKIP (RTSI Skip)

This attribute defines the number of RTSI events to skip before logging them to the read queue for that object. Use this attribute with `NC_ATTR_RTSSI_MODE` and an attribute value of `NC_RTSSI_TIME_ON_IN`.

Attribute values: Any user number.

Examples

The following examples are available:

- C programming (in the `\\nican\examples\CAN-DAQ Synchronization` folder)

CAN Master functionality is shown in the following examples:

- Network Interface controls RTSI on CAN
`Transmit.cpp`
- Network Interface controls RTSI manually.`cpp`
- CAN Object controls RTSI on Unsolicited
`Receive.cpp`

CAN Slave (DAQ Master) functionality is shown in the following examples:

- Network Interface transmits CAN frame on RTSI.cpp
- Network Interface Read Queue receives time stamp on RTSI.cpp
- CAN Object Read Queue receives time stamp on RTSI.cpp
- LabVIEW programming (in `\\your LV folder\Examples\nican`)

CAN Master functionality is shown in the following examples:

- Network Interface controls RTSI on ncAction.vi
- Network Interface controls RTSI on CAN Receive.vi
- Network Interface controls RTSI on CAN Transmit.vi
- CAN Object controls RTSI on ncAction.vi
- CAN Object controls RTSI on Periodic Transmit.vi
- CAN Object controls RTSI on Unsolicited Receive.vi
- CAN Object controls RTSI on Waveform Transmit.vi

CAN Slave (DAQ Master) functionality is shown in the following examples:

- Network Interface Read Queue receives time stamp on RTSI.vi
- Network Interface transmits CAN frame on RTSI.vi
- CAN Object Read Queue receives time stamp on RTSI.vi
- CAN Object transmits Periodic on RTSI.vi
- CAN Object transmit Waveform on RTSI.vi

For information about using the examples and which tester to use on the DAQ board to test the functionality, refer to documentation in the C source file and VI-Info (for LabVIEW examples).

NI-CAN Object States

This appendix describes the NI-CAN object states.

Every object in NI-CAN contains a state attribute (`NC_ATTR_STATE`) with the following format. The bits marked as 0 are reserved for future use.

31-6	5	4	3	2	1	0
0	WARNING	ERROR	0	STOPPED	WRITE SUCCESS	READ AVAIL

Figure A-1. State Format

You can detect the object states using one of the following schemes:

- Call `ncGetAttribute` to get the `NC_ATTR_STATE` attribute.
- Call `ncWaitForState` to wait for one or more states to occur.
- Use `ncCreateNotification` to register a callback for one or more states.

Table A-1 describes each object state.

Table A-1. NI-CAN Object States

Constant	Bitmask (Hex)	Description
<code>NC_ST_READ_AVAIL</code>	00000001 (Bit 0)	Indicates that new data is available to be read using <code>ncRead</code> . Set when data is received from network, and cleared when all available data is read.
<code>NC_ST_WRITE_SUCCESS</code>	00000002 (Bit 1)	Indicates that all data provided using <code>ncWrite</code> has been successfully transmitted onto network. Set when last transmission is successful, and cleared by any call to <code>ncWrite</code> .

Table A-1. NI-CAN Object States (Continued)

Constant	Bitmask (Hex)	Description
NC_ST_STOPPED	00000004 (Bit 2)	Indicates that object is in stopped state (not communicating on network). This state can occur as result of calling <code>ncAction</code> with <code>NC_OP_STOP</code> , or due to serious communication error, such as CAN bus off, which causes object to stop. If this state is clear, the object is in its normal running state.
NC_ST_ERROR	00000010 (Bit 4)	Indicates that an error status has occurred in background. Set when error occurs, and cleared when you obtain status value. Status value is obtained by getting <code>NC_ATTR_STATUS</code> attribute, or on next call to <code>ncRead</code> or <code>ncWrite</code> . This state indicates background problems such as communication errors, and is not set for problems that are associated with individual function calls (such as an invalid parameter).
NC_ST_WARNING	00000020 (Bit 5)	Indicates that warning status has occurred in background. Set when warning occurs, and cleared when you obtain status value. Status value is obtained by getting <code>NC_ATTR_STATUS</code> attribute, or on next call to <code>ncRead</code> or <code>ncWrite</code> . This state indicates background problems such as communication warnings, and is not set for problems that are associated with individual function calls (such as an invalid parameter).

Status Codes and Qualifiers

This appendix describes the NI-CAN status codes and the qualifiers for each code.

Each NI-CAN function returns a value that indicates the status of the function call. Your application should check this status after each NI-CAN function call. The following sections describe the NI-CAN status.

NI-CAN Status Format

To provide the maximum amount of information, the status returned by NI-CAN functions is encoded as a signed 32-bit integer. The format of this integer is shown in Figure B-1.

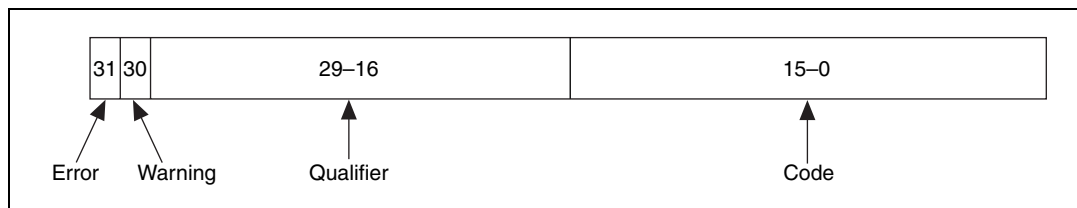


Figure B-1. Status Format

Error/Warning Indicators (Severity)

The error and warning bits ensure that all NI-CAN errors generate a negative status, and all NI-CAN warnings generate a positive status. The error bit is set when a function does not perform the expected behavior, resulting in a negative status. The warning bit is set when the function performed as expected, but a condition exists that may require your attention. If no error or warning occurs, the entire status is set to zero to indicate success. Table B-1 summarizes the behavior of NI-CAN status.

Table B-1. Determining Severity of Status

Status	Result
Negative	Error. Function did not perform expected behavior.
Zero	Success. Function completed successfully.
Positive	Warning. Function performed as expected, but a condition arose that may require your attention.

Code

The code bits indicate the primary status code used for warning or errors.

Qualifier

The qualifier bits hold a qualifier for the warning or error code. It is specific to individual values for the code field, and provides additional information useful for detailed debugging. For example, if the status code indicates an invalid function parameter, the qualifier holds a number which indicates the exact parameter that is invalid (one for the first parameter, two for the second, and so on). If no qualifier exists, this field has the value `NC_QUAL_NONE (0)`.

Checking Status in LabVIEW

For applications written in G (LabVIEW), status checking is basically handled automatically. For all of the NI-CAN functions, the lower left and right terminals provide status information using LabVIEW Error Clusters. LabVIEW Error Clusters are designed so that status information flows from one function to the next, and function execution stops when an error occurs. For more information, refer to the *Error Handling* section in the LabVIEW Online Reference.

In the NI-CAN implementation of Error Clusters, the `status` parameter is set to true when an error occurs, and is set to false when a warning or success occurs. The `code` parameter of the Error Cluster contains the code and qualifier fields of the NI-CAN status. If the `code` parameter of the Error Cluster is not zero, then a warning or error was detected. When the `status` parameter is true, the `source` parameter of the Error Cluster provides the name of the NI-CAN function in which the error occurred.

Within your LabVIEW Block Diagram, wire the `Error in` and `Error out` terminals of all NI-CAN functions together in succession. When an error is detected in any NI-CAN function (`status` parameter true), all

subsequent NI-CAN functions are skipped except for `ncClose`. The `ncClose` function executes regardless of whether the incoming `status` is true or false. This ensures that all NI-CAN objects are closed properly when execution stops due to an error.

When a warning occurs in an NI-CAN function, execution proceeds normally. To detect suspected warnings in your application, you can write code in your Block Diagram to examine the `code` parameter, or you can use the Probe Data tool on an Error out terminal during execution.

For each NI-CAN function, you can find numeric values for the returned status code and qualifier in the online description of the function, which you can access in the Block Diagram by selecting the function and typing <Ctrl-H>.

Checking Status in C

For applications written in C or C++, you should define a function to handle NI-CAN warnings and errors. When this function detects an error, it closes all open objects, then exits the application. When this function detects a warning, it can display a warning message or simply ignore the warning. If the function has the following prototype:

```
void CheckStat(NCTYPE_STATUS stat, char *msg);
```

then your application invokes it as follows:

```
if (status != 0)
    CheckStat(status, "NI-CAN error or warning");
```

For an example implementation of the `CheckStat` function, refer to the C language examples in the NI-CAN `examples` directory.

When accessing the NI-CAN code and qualifier within your application, you should use the constants defined in `nican.h`. These constants have the same names as described later in this appendix. For example, to check for a timeout, you would use code such as the following:

```
if (NC_STATCODE(status) == NC_ERR_TIMEOUT)
    printf("NI-CAN timeout");
```

NI-CAN Status Codes and Qualifiers

Table B-2 summarizes each NI-CAN status code (lower 16 bits of status). After the table, a separate section for each status code lists the valid encodings for the entire status, including the associated qualifier and severity.

Table B-2. Summary of Status Codes

Code	Hex Encoding of Code (Lower 16 Bits)	Description
NC_SUCCESS	0000	Success (no warning or error)
NC_ERR_TIMEOUT	0001	Timeout Expired
NC_ERR_DRIVER	0002	Implementation-specific error in NI-CAN driver
NC_ERR_BAD_NAME	0003	Invalid or unrecognized object name
NC_ERR_BAD_PARAM	0004	Invalid function parameter
NC_ERR_BAD_VALUE	0005	Invalid attribute value
NC_ERR_ALREADY_OPEN	0006	Object already opened by another application
NC_ERR_NOT_STOPPED	0007	Attempted to set a configuration attribute while object was running
NC_ERR_OVERFLOW	0008	Queue overflow
NC_ERR_OLD_DATA	0009	Data returned from <code>ncRead</code> matches data returned from previous call to <code>ncRead</code>
NC_ERR_CAN_BUS_OFF	0101	Error or warning indicating large number of CAN communication errors

NC_SUCCESS (0000 Hex)

Success (no warning or error).

Hex Status Encoding 00000000

Qualifier	0
Severity	Success
Description	The qualifier is always zero.

NC_ERR_TIMEOUT (0001 Hex)

A timeout expired in the NI-CAN driver. The qualifier indicates the type of timeout that expired.

Hex Status Encoding 80000001

Qualifier	NC_QUAL_TIMO_FUNCTION (0)
Severity	Error
Description	The timeout of <code>ncWaitForState</code> or <code>ncCreateNotification</code> expired before any desired states occurred.
Solutions	<ul style="list-style-type: none"> • Increase the value of the <code>Timeout</code> parameter to wait longer. • If the timeout occurs while waiting for <code>NC_ST_READ_AVAIL</code> or <code>NC_ST_WRITE_SUCCESS</code>, verify your CAN cable connections, and ensure that remote devices are operating properly. • If you wait only for a background error or warning, the timeout is often the expected behavior, and you can ignore it.

Hex Status Encoding 80010001

Qualifier	NC_QUAL_TIMO_WATCHDOG (1)
Severity	Error
Description	The watchdog timeout for a CAN Object expired, indicating that data was not received at the rate expected. This error occurs in the background and is returned by <code>ncRead</code> and <code>ncWrite</code> .
Solutions	Verify your CAN cable connections, and ensure that remote devices are operating properly. If the remote device takes longer than expected to transmit data, you can increase the period specified in the <code>NC_ATTR_BKD_PERIOD</code> attribute.

NC_ERR_DRIVER (0002 Hex)

An implementation-specific error has occurred in the NI-CAN driver, such as the inability to allocate needed memory. This error should never occur under normal circumstances.

Hex Status Encoding 8xxx0002, 9xxx0002, Axxx0002, and Bxxx0002

Qualifier	Varies
Severity	Error
Description	The qualifier (bits 16-29) holds a value that is specific to the NI-CAN driver implementation.
Solutions	Write down the status value, and contact National Instruments for technical support.

NC_ERR_BAD_NAME (0003 Hex)

The `ObjName` parameter of `ncOpenObject` or `ncConfig` contains an invalid or unrecognized name.

Hex Status Encoding 80000003

Qualifier	0
Severity	Error
Description	There is a basic syntax error such as an invalid character or a single colon instead of a double colon.
Solutions	<ul style="list-style-type: none"> • Verify that the object name does not contain invalid characters, and that you use the syntax specified in <code>ncOpenObject</code>. • If you are opening a user-defined alias, use the NI-CAN Configuration utility to verify that the alias is defined in the list of CAN Objects.

Hex Status Encoding 80010003

Qualifier	1
Severity	Error
Description	The CAN Network Interface Object name is invalid or unknown.
Solutions	Use the NI-CAN Configuration utility to verify that the CAN Network Interface Object is assigned a physical CAN port. The NI-CAN Diagnostic utility also provides a list of valid CAN Network Interface Object names.

Hex Status Encoding 80020003

Qualifier	1
Severity	Error
Description	The CAN Object name is invalid or unknown.
Solutions	Verify that you use the syntax specified in the <i>CAN Object</i> section of Chapter 3, <i>NI-CAN Objects</i> .

NC_ERR_BAD_PARAM (0004 Hex)

A function parameter is invalid.

Hex Status Encoding 800x0004

Qualifier	Varies
Severity	Error
Description	The qualifier holds the position of the invalid parameter in the C function prototype. For example, if the <code>DataSize</code> parameter of <code>ncRead</code> is invalid, the qualifier is two (status 80020004).
Solutions	Check the qualifier, then read the function description in Chapter 2, <i>NI-CAN Functions</i> , to verify that you provide a valid value for the specified parameter.

NC_ERR_BAD_VALUE (0005 Hex)

The attribute value for the specified attribute ID is invalid. For example, if you call `ncSetAttribute` with the `AttrId` `NC_ATTR_BAUD_RATE`, and `AttrPtr` points to an invalid baud rate such as 20005, `NC_ERR_BAD_VALUE` is returned.

Hex Status Encoding 80000005

Qualifier	0 (for <code>ncSetAttribute</code>)
Severity	Error
Description	For <code>ncSetAttribute</code> , the qualifier is always zero.
Solutions	Check the description of the attribute in Chapter 3, <i>NI-CAN Objects</i> , and verify that the value you pass is valid.

Hex Status Encoding 8xxx0005

Qualifier	Varies (for <code>ncAction</code> and <code>ncConfig</code>)
Severity	Error
Description	For <code>ncAction</code> and <code>ncConfig</code> , this error indicates that although each configuration attribute holds a valid value, the combination of values is invalid. For example, if a CAN Object is configured as Transmit Value Periodically, the period attribute must be nonzero. For this error, the qualifier holds the low order bits of the <code>AttrId</code> of one of the invalid attributes.
Solutions	Using the attribute ID provided in the qualifier, check the description of the attribute in Chapter 3, <i>NI-CAN Objects</i> , and verify that the value you set works with the other attribute values.

NC_ERR_ALREADY_OPEN (0006 Hex)

The object has already been opened by another application. If one application opens an object, no other application can open or configure that object until the object is closed.

Hex Status Encoding 80000006

Qualifier	0
Severity	Error
Description	The qualifier is always zero.
Solutions	<ul style="list-style-type: none"> • If you have two or more applications that open the same object, run only one application at a time. • If two or more applications need to share an object, you can alternate access by closing the object in one application, then opening the object in another. • Before exiting your application, verify that you call <code>ncCloseObject</code> for every object opened. For LabVIEW, you should implement a control on your front panel to stop the program and close all objects. You should not use the LabVIEW Stop button to stop execution, because doing so often prevents proper use of <code>ncCloseObject</code>.

NC_ERR_NOT_STOPPED (0007 Hex)

You attempted to set a configuration attribute for an object while the object was running. You can change attributes with `Config` permissions only when the object is stopped (not communicating).

Hex Status Encoding 80000007

Qualifier	0
Severity	Error
Description	The qualifier is always zero.
Solutions	<ul style="list-style-type: none"> • Configure the object prior to opening it, either within the NI-CAN Configuration utility, or by using <code>ncConfig</code>. • Use <code>ncAction</code> to stop and start communication as needed so that you can update configuration attributes.

NC_ERR_OVERFLOW (0008 Hex)

There is a queue overflow.

Hex Status Encoding 80000008

Qualifier	NC_QUAL_OVFL_WRITE
Severity	Error
Description	There is a write queue overflow. This error occurs when you call <code>ncWrite</code> for a full write queue. It occurs only when the length of the write queue is greater than zero.
Solutions	<ul style="list-style-type: none"> • Increase the length of the write queue using the <code>NC_ATTR_WRITE_Q_LEN</code> attribute. • Prior to calling <code>ncWrite</code>, check <code>NC_ATTR_WRITE_PENDING</code> to verify that it is less than the write queue length. • If you merely want the most recent data to be transmitted, such as for periodic transmission, set <code>NC_ATTR_WRITE_Q_LEN</code> to zero. • Wait for the <code>NC_ST_WRITE_SUCCESS</code> state before calling <code>ncWrite</code> to queue more data.

Hex Status Encoding 80010008

Qualifier	NC_QUAL_OVFL_READ
Severity	Error
Description	There is a read queue overflow. This error occurs when new data is received from the network for a full read queue, and NI-CAN discards it. The error occurs only when the length of the read queue is greater than zero. This error occurs in the background, and is returned by <code>ncRead</code> and <code>ncWrite</code> .
Solutions	<ul style="list-style-type: none"> • Increase the length of the read queue using the <code>NC_ATTR_READ_Q_LEN</code> attribute. • Call <code>ncRead</code> more often in your application. One way to do this is to create a notification for <code>NC_ST_READ_AVAIL</code> using <code>ncCreateNotification</code>, so that you can read data as soon as it becomes available. • If you merely want the most recent data from <code>ncRead</code>, set <code>NC_ATTR_READ_Q_LEN</code> to zero. • Check <code>NC_ATTR_READ_PENDING</code> for a given threshold prior to calling <code>ncRead</code>.

Hex Status Encoding 80020008

Qualifier	NC_QUAL_OVFL_CHIP
Severity	Error
Description	There is an overflow in the CAN communications controller chip. This error occurs in the background and is returned by <code>ncRead</code> and <code>ncWrite</code> .
Solutions	Disable timestamping by setting the <code>NC_ATTR_TIMESTAMPING</code> attribute to <code>NC_FALSE</code> .

NC_ERR_OLD_DATA (0009 Hex)

The data returned from `ncRead` matches the data returned from the previous call to `ncRead`. Because the old data is returned successfully, this status code has a warning severity, not error.

Hex Status Encoding 40000009

Qualifier	0
Severity	Warning
Description	The qualifier is always zero.
Solutions	<ul style="list-style-type: none"> • If you merely want to read the most recent data, ignore this warning. • Wait for the <code>NC_ST_READ_AVAIL</code> state before calling <code>ncRead</code>.

NC_ERR_CAN_BUS_OFF (0101 Hex)

This is an error or warning that can indicate many different CAN communication errors. When the transmit or receive error counter of the CAN communications controller chip increments above 96, a warning occurs. When the transmit error counter increments above 255 (bus off), an error occurs and the network interface is stopped. In both cases the qualifier is set to the most recent detected communication error. This warning/error occurs in the background, and is returned by `ncRead` and `ncWrite`. For more information, refer to the [CAN Network Interface Object](#) section of Chapter 3, *NI-CAN Objects*.

The solutions for all of the qualifiers of the NC_ERR_CAN_BUS_OFF error follow the descriptions.

Hex Status Encoding 40010101 and 80010101

Qualifier	NC_QUAL_CAN_STUFF
Severity	Varies
Description	A stuff error has occurred (more than five equal bits in the frame).

Hex Status Encoding 40020101 and 80020101

Qualifier	NC_QUAL_CAN_FORM
Severity	Varies
Description	The frame format is wrong.

Hex Status Encoding 40030101 and 80030101

Qualifier	NC_QUAL_CAN_ACK
Severity	Varies
Description	The frame has not been acknowledged.

Hex Status Encoding 40040101 and 80040101

Qualifier	NC_QUAL_CAN_BIT1
Severity	Varies
Description	One was transmitted but zero was detected.

Hex Status Encoding 40050101 and 80050101

Qualifier	NC_QUAL_CAN_BIT0
Severity	Varies
Description	Zero was transmitted but one was detected.

Hex Status Encoding 40060101 and 80060101

Qualifier	NC_QUAL_CAN_CRC
Severity	Varies
Description	The CRC checksum is invalid.

Solutions

The following solutions apply to all of the qualifiers for the NC_ERR_CAN_BUS_OFF error:

- CAN communication errors are often caused by defective cabling. Verify that your connector, cables, and devices are functioning properly.
- If you attempt to transmit a CAN frame without another CAN device connected, or with the bus powered off, the NC_ERR_CAN_BUS_OFF warning occurs. Connect your other CAN devices prior to attempting communication.



Technical Support Resources

Web Support

National Instruments Web support is your first stop for help in solving installation, configuration, and application problems and questions. Online problem-solving and diagnostic resources include frequently asked questions, knowledge bases, product-specific troubleshooting wizards, manuals, drivers, software updates, and more. Web support is available through the Technical Support section of ni.com

NI Developer Zone

The NI Developer Zone at ni.com/zone is the essential resource for building measurement and automation systems. At the NI Developer Zone, you can easily access the latest example programs, system configurators, tutorials, technical news, as well as a community of developers ready to share their own techniques.

Customer Education

National Instruments provides a number of alternatives to satisfy your training needs, from self-paced tutorials, videos, and interactive CDs to instructor-led hands-on courses at locations around the world. Visit the Customer Education section of ni.com for online course schedules, syllabi, training centers, and class registration.

System Integration

If you have time constraints, limited in-house technical resources, or other dilemmas, you may prefer to employ consulting or system integration services. You can rely on the expertise available through our worldwide network of Alliance Program members. To find out more about our Alliance system integration solutions, visit the System Integration section of ni.com

Worldwide Support

National Instruments has offices located around the world to help address your support needs. You can access our branch office Web sites from the Worldwide Offices section of ni.com. Branch office Web sites provide up-to-date contact information, support phone numbers, e-mail addresses, and current events.

If you have searched the technical support resources on our Web site and still cannot find the answers you need, contact your local office or National Instruments corporate. Phone numbers for our worldwide offices are listed at the front of this manual.

Glossary

Prefix	Meanings	Value
n-	nano-	10^{-9}
m-	milli-	10^{-3}
k-	kilo-	10^3
M-	mega-	10^6

A

action *See* [method](#).

actuator A device that uses electrical, mechanical, or other signals to change the value of an external, real-world variable. In the context of device networks, actuators are devices that receive their primary data value from over the network; examples include valves and motor starters. Also known as *final control element*.

Application Programming Interface (API) A collection of functions used by a user application to access hardware. Within NI-CAN, you use API functions to make calls into the NI-CAN driver.

arbitration ID An 11- or 29-bit ID transmitted as the first field of a CAN frame. The arbitration ID determines the priority of the frame, and is normally used to identify the data transmitted in the frame.

attribute The externally visible qualities of an object; for example, an instance Mary of class Human could have the attributes Gender and Age, with the values Female and 31. Also known as *property*.

B

b	Bits.
bus off	A CAN node goes into the bus off state when its transmit error counter increments above 255. The node does not participate in network traffic, because it assumes that a defect exists that must be corrected.

C

CAN	Controller Area Network.
CAN/LS	See Low-speed CAN .
CAN data frame	Frame used to transmit the actual data of a CAN Object. The RTR bit is clear, and the data length indicates the number of data bytes in the frame.
CAN frame	In addition to fields used for error detection/correction, a CAN frame consists of an arbitration ID, the RTR bit, a four-bit data length, and zero to eight bytes of data.
CAN Network Interface Object	Within NI-CAN, an object that encapsulates a CAN network interface on the host computer.
CAN Object	A CAN identifier, along with its associated data.
CAN remote frame	Frame used to request data for a CAN Object from a remote node; the RTR bit is set, and the data length indicates the amount of data desired (but no data bytes are included).
class	A set of objects that share a common structure and a common behavior.
connection	An association between two or more nodes on a network that describes when and how data is transferred.
controller	A device that receives data from sensors and sends data to actuators in order to hold one or more external, real-world variables at a certain level or condition. A thermostat is a simple example of a controller.

D

device	See node .
device network	Multi-drop digital communication network for sensors, actuators, and controllers.
DLL	Dynamic link library.
DMA	Direct memory access.

E

error active	A CAN node is in error active state when both the receive and transmit error counters are below 128.
error counters	Every CAN node keeps a count of how many receive and transmit errors have occurred. The rules for how these counters are incremented and decremented are defined by the CAN protocol specification.
error passive	A CAN node is in error passive state when one or both of its error counters increment above 127. This state is a warning that a communication problem exists, but the node is still participating in network traffic.
extended arbitration ID	A 29-bit arbitration ID. Frames that use extended IDs are often referred to as CAN 2.0 Part B (the specification that defines them).

F

FCC	Federal Communications Commission.
frame	A unit of information transferred across a network from one node to another; the protocol defines the meaning of the bit fields within a frame. Also known as <i>packet</i> .

H

hex	Hexadecimal.
Hz	Hertz.

I

instance An abstraction of a specific real-world thing; for example, Mary is an instance of the class Human. Also known as *object*.

ISO International Standards Organization.

K

KB Kilobytes of memory.

L

LabVIEW Laboratory Virtual Instrument Engineering Workbench.

local Within NI-CAN, anything that exists on the same host (personal computer) as the NI-CAN driver.

Low-speed CAN Implementation of CAN as defined in ISO 11519.

M

MB Megabytes of memory.

method An action performed on an instance to affect its behavior; the externally visible code of an object. Within NI-CAN, you use NI-CAN functions to execute methods for objects. Also known as *service*, *operation*, and *action*.

minimum interval For a given connection, the minimum amount of time between subsequent attempts to transmit frames on the connection. Some protocols use minimum intervals to guarantee a certain level of overall network performance.

multi-drop A physical connection in which multiple devices communicate with one another along a single cable.

N

network interface	A node's physical connection onto a network.
NI-CAN driver	Device driver and/or firmware that implement all the specifics of a CAN network interface. Within NI-CAN, this software implements the CAN Network Interface Object as well as all objects above it in the object hierarchy.
node	A physical assembly, linked to a communication line (cable), capable of communicating across the network according to a protocol specification. Also known as <i>device</i> .
notification	Within NI-CAN, an operating system mechanism that the NI-CAN driver uses to communicate events to your application. You can think of a notification of as an API function, but in the opposite direction.

O

object	See instance .
object-oriented	A software design methodology in which classes, instances, attributes, and methods are used to hide all of the details of a software entity that do not contribute to its essential characteristics.

P

peer-to-peer	Network connection in which data is transmitted from the source to its destination(s) without need for an explicit request. Although data transfer is generally unidirectional, the protocol often uses low level acknowledgments and error detection to ensure successful delivery.
periodic	Connections that transfer data on the network at a specific rate.
polled	Request/response connection in which a request for data is sent to a device, and the device sends back a response with the desired value.
protocol	A formal set of conventions or rules for the exchange of information among nodes of a given network.

R

RAM	Random-access memory.
remote	Within NI-CAN, anything that exists in another node of the device network (not on the same host as the NI-CAN driver).
Remote Transmission Request (RTR) bit	This bit follows the arbitration ID in a frame, and indicates whether the frame is the actual data of the CAN Object (CAN data frame), or whether the frame is a request for the data (CAN remote frame).
request/response	Network connection in which a request is transmitted to one or more destination nodes, and those nodes send a response back to the requesting node. In industrial applications, the responding (slave) device is usually a sensor or actuator, and the requesting (master) device is usually a controller. Also known as <i>master/slave</i> .
resource	Hardware settings used by National Instruments CAN hardware, including an interrupt request level (IRQ) and an 8 KB physical memory range (such as D0000 to D1FFF hex).

S

s	Seconds.
sensor	A device that measures electrical, mechanical, or other signals from an external, real-world variable; in the context of device networks, sensors are devices that send their primary data value onto the network; examples include temperature sensors and presence sensors. Also known as <i>transmitter</i> .
standard arbitration ID	An 11-bit arbitration ID. Frames that use standard IDs are often referred to as CAN 2.0 Part A; standard IDs are by far the most commonly used.

U

unsolicited	Connections that transmit data on the network sporadically based on an external event. Also known as <i>nonperiodic</i> , <i>sporadic</i> , and <i>event driven</i> .
-------------	-----------------------------------------------------------------------------------------------------------------------------------------------------------------------

V

VI Virtual Instrument.

W

watchdog timeout A timeout associated with a connection that expects to receive network data at a specific rate. If data is not received before the watchdog timeout expires, the connection is normally stopped. You can use watchdog timeouts to verify that the remote node is still operational.

Index

A

attributes

See CAN Network Interface Object.

See CAN Object.

See RTSI programming.

B

bus off states, CAN Network Interface Object, 3-3

C

C/C++ applications, status checking, B-3

callback. *See* ncCreateNotification function.

CAN Network Interface Object, 3-2

attributes, 3-4

NC_ATTR_ABS_TIME, 3-4

NC_ATTR_BAUD_RATE, 3-4

NC_ATTR_CAN_COMP_STD, 3-5

NC_ATTR_CAN_COMP_XTD, 3-6

NC_ATTR_CAN_MASK_STD, 3-6

NC_ATTR_CAN_MASK_XTD, 3-7

NC_ATTR_LOG_COMM_ ERRS, 3-12

NC_ATTR_PROTOCOL, 3-7

NC_ATTR_PROTOCOL_ VERSION, 3-7

NC_ATTR_READ_MULT_ SIZE, 3-13

NC_ATTR_READ_PENDING, 3-8

NC_ATTR_READ_Q_LEN, 3-8

NC_ATTR_RSTI_SKIP, 3-17

NC_ATTR_RTSI_MODE, 3-13

NC_ATTR_RTSI_SIG_BEHAV, 3-16

NC_ATTR_RTSI_SIGNAL, 3-16

NC_ATTR_RX_Q_LEN, 3-11

NC_ATTR_SOFTWARE_ VERSION, 3-8

NC_ATTR_START_ON_OPEN, 3-9

NC_ATTR_STATE, 3-9

NC_ATTR_STATUS, 3-10

NC_ATTR_WRITE_PENDING, 3-10

NC_ATTR_WRITE_Q_LEN, 3-10

description, 3-2

encapsulates, 3-2

error active, error passive, and bus off states, 3-3

object name, 3-2

CAN Object, 3-17

attributes, 3-18

NC_ATTR_CAN_DATA_ LENGTH, 3-18

NC_ATTR_CAN_TX_ RESPONSE, 3-18

NC_ATTR_COMM_TYPE, 3-19

NC_ATTR_PERIOD, 3-19

NC_ATTR_READ_MULT_ SIZE, 3-21

NC_ATTR_READ_PENDING, 3-20

NC_ATTR_READ_Q_LEN, 3-20

NC_ATTR_RTSI_FRAME, 3-25

NC_ATTR_RTSI_MODE, 3-21

NC_ATTR_RTSI_SIG_BEHAV, 3-24

NC_ATTR_RTSI_SIGNAL, 3-24

NC_ATTR_RTSI_SKIP, 3-25

NC_ATTR_RX_CHANGES_ ONLY, 3-26

NC_ATTR_STATE, 3-26

NC_ATTR_STATUS, 3-27

NC_ATTR_WRITE_PENDING, 3-27

NC_ATTR_WRITE_Q_LEN, 3-27

- communication type values, 3-28
 - Receive Periodically Using Remote (NC_CAN_COMM_RX_PERIODIC), 3-28
 - Receive Unsolicited (NC_CAN_COMM_RX_UN SOL), 3-28
 - Receive Value by Call Using Remote (NC_CAN_COMM_RX_BY_CALL), 3-29
 - Transmit Data by Call (NC_CAN_COMM_TX_BY_CALL), 3-30
 - Transmit Data Periodically (NC_CAN_COMM_TX_PERIODIC), 3-29
 - Transmit Periodic Waveform (NC_CAN_COMM_TX_WAVEFORM), 3-31
 - Transmit Value by Response Only (NC_CAN_COMM_TX_RESP_ONLY), 3-30
 - description, 3-17
 - encapsulates, 3-17
 - object name, 3-17
 - code, NI-CAN status format, B-2
 - communication type attribute (NC_ATTR_COMM_TYPE), 3-19
 - communication type examples, 3-32
 - periodic polling of remote data (figure), 3-33
 - periodic transmission (figure), 3-32
 - polling remote data using ncWrite (figure), 3-32
 - communication type values
 - Receive Periodically Using Remote (NC_CAN_COMM_RX_PERIODIC), 3-28
 - Receive Unsolicited (NC_CAN_COMM_RX_UN SOL), 3-28
 - Transmit Data Periodically (NC_CAN_COMM_TX_PERIODIC), 3-29
 - Transmit Periodic Waveform (NC_CAN_COMM_TX_WAVEFORM), 3-31
 - Transmit Value by Response Only (NC_CAN_COMM_TX_RESP_ONLY), 3-30
 - conventions used in this manual, *xi*
 - customer education, C-1
- ## D
- data types, NI-CAN host (table), 1-1
- ## E
- error active, CAN Network Interface Object, 3-3
 - error passive, CAN Network Interface Object, 3-3
 - error warning indicators (severity), B-1
 - example of periodic transmission (figure), 3-32
- ## F
- functions. *See* NI-CAN functions.
- ## G
- glossary of terms, G-1
- ## H
- how to use this manual set, *xi*
- ## L
- LabVIEW applications, status checking, B-2

M

manual set, how to use, *xi*

N

National Instruments Web support, C-1

NC_ATTR_ABS_TIME, 3-4

NC_ATTR_BAUD_RATE, 3-4

NC_ATTR_CAN_COMP_STD, 3-5

NC_ATTR_CAN_COMP_XTD, 3-6

NC_ATTR_CAN_DATA_LENGTH, 3-18

NC_ATTR_CAN_MASK_STD, 3-6

NC_ATTR_CAN_MASK_XTD, 3-7

NC_ATTR_CAN_TX_RESPONSE, 3-18

NC_ATTR_COMM_TYPE, 3-19

See also communication type values.

NC_ATTR_LOG_COMM_ERRS, 3-12

NC_ATTR_PERIOD, 3-19

NC_ATTR_PROTOCOL, 3-7

NC_ATTR_PROTOCOL_VERSION, 3-7

NC_ATTR_READ_MULT_SIZE, 3-13, 3-21

NC_ATTR_READ_PENDING

CAN Network Interface Object, 3-8

CAN Object, 3-20

NC_ATTR_READ_Q_LEN

CAN Network Interface Object, 3-8

CAN Object, 3-20

NC_ATTR_RTSI_FRAME, 3-25, 4-5

NC_ATTR_RTSI_MODE, 3-13, 3-21, 4-2

NC_ATTR_RTSI_SIG_BEHAV, 3-16,
3-24, 4-4

NC_ATTR_RTSI_SIGNAL, 3-16, 3-24

NC_ATTR_RTSI_SIGNAL (RTSI Line
Number), 4-4

NC_ATTR_RTSI_SKIP, 3-17, 3-25, 4-5

NC_ATTR_RX_CHANGES_ONLY, 3-26

NC_ATTR_RX_Q_LEN, 3-11

NC_ATTR_SOFTWARE_VERSION, 3-8

NC_ATTR_START_ON_OPEN, 3-9

NC_ATTR_STATE

CAN Network Interface Object, 3-9

CAN Object, 3-26

NC_ATTR_STATUS

CAN Network Interface Object, 3-10

CAN Object, 3-27

NC_ATTR_WRITE_PENDING

CAN Network Interface Object, 3-10

CAN Object, 3-27

NC_ATTR_WRITE_Q_LEN

CAN Network Interface Object, 3-10

CAN Object, 3-27

NC_ERR_ALREADY_OPEN (0006 Hex)

status code, B-9

NC_ERR_BAD_NAME (0003 Hex) status

code, B-7

NC_ERR_BAD_PARAM (0004 Hex) status

code, B-7

NC_ERR_BAD_VALUE (0005 Hex) status

code, B-8

NC_ERR_CAN_BUS_OFF (0101 Hex) status

code, B-11

NC_ERR_DRIVER (0002 Hex) status

code, B-6

NC_ERR_NOT_STOPPED (0007 Hex) status

code, B-9

NC_ERR_OLD_DATA (0009 Hex) status

code, B-11

NC_ERR_OVERFLOW (0008 Hex) status

code, B-9

NC_ERR_TIMEOUT (0001 Hex) status

code, B-5

NC_RTSI_NONE (Disable RTSI), 4-2

NC_RTSI_OUT_ACTION_ONLY (RTSI

Output on ncAction call), 4-4

NC_RTSI_OUT_ON_RX (RTSI Output on

Receiving CAN frame), 4-3

NC_RTSI_OUT_ON_TX (RTSI Output on

Transmitting CAN frame), 4-4

NC_RTSI_TIME_ON_IN (On RTSI

Input—Timestamp RTSI event), 4-3

- NC_RTSM_TX_ON_IN (On RTSM
Input—Transmit CAN Frame), 4-2
- NC_SUCCESS (0000 Hex) status code, B-5
- ncAction function, 2-3
 - CAN Network Interface Object, 2-4
 - actions supported (table), 2-4
 - CAN Object, 2-5
 - actions supported (table), 2-5
 - description, 2-3
 - example, 2-5
 - format, 2-3
 - input, 2-3
 - purpose, 2-3
 - return status, 2-5
- ncCloseObject function, 2-6
 - CAN Network Interface Object, 2-6
 - CAN Object, 2-6
 - description, 2-6
 - example, 2-6
 - format, 2-6
 - input, 2-6
 - purpose, 2-6
 - return status, 2-6
- ncConfig function, 2-7
 - CAN Network Interface Object, 2-9
 - CAN Object, 2-9
 - description, 2-8
 - using the LabVIEW configuration functions, 2-8
 - example, 2-10
 - format, 2-7
 - input, 2-8
 - purpose, 2-7
 - return status, 2-10
- ncCreateNotification function, 2-12
 - callback description, 2-14
 - callback parameters, 2-13
 - callback prototype, 2-13
 - callback return value, 2-13
 - CAN Network Interface Object, 2-14
 - CAN Object, 2-15
 - description, 2-12
 - example, 2-15
 - format, 2-12
 - input, 2-12
 - purpose, 2-12
 - return status, 2-15
- ncCreateOccurrence function, 2-17
 - CAN Network Interface Object, 2-18
 - CAN Object, 2-18
 - description, 2-17
 - example, 2-19
 - format, 2-17
 - input, 2-17
 - output, 2-17
 - purpose, 2-17
 - return status, 2-18
- ncGetAttribute function, 2-20
 - CAN Network Interface Object, 2-21
 - CAN Object, 2-21
 - description, 2-20
 - example, 2-21
 - format, 2-20
 - input, 2-20
 - output, 2-20
 - purpose, 2-20
 - return status, 2-21
- ncOpenObject function, 2-22
 - CAN Network Interface Object, 2-23
 - CAN Object, 2-23
 - description, 2-22
 - examples, 2-24
 - format, 2-22
 - input, 2-22
 - output, 2-22
 - purpose, 2-22
 - return status, 2-23

- ncRead function, 2-25
 - CAN Network Interface Object, 2-27
 - NCTYPE_CAN_FRAME_TIMED field names (table), 2-27
 - CAN Object, 2-28
 - NCTYPE_CAN_DATA_TIMED field names (table), 2-29
 - description, 2-26
 - examples, 2-29
 - format, 2-25
 - input, 2-25
 - output, 2-25
 - purpose, 2-25
 - return status, 2-29
- ncReadMult function, 2-30
 - description, 2-30
 - examples, 2-32
 - format, 2-30
 - input, 2-30
 - output, 2-30
 - purpose, 2-30
 - return status, 2-31
- ncReset function, 2-33
 - description, 2-33
 - format, 2-33
 - input, 2-33
 - purpose, 2-33
- ncSetAttribute function, 2-34
 - CAN Network Interface Object, 2-35
 - CAN Object, 2-35
 - description, 2-34
 - example, 2-35
 - format, 2-34
 - input, 2-34
 - purpose, 2-34
 - return status, 2-35
- NCTYPE_CAN_DATA field names (table), 2-40
- NCTYPE_CAN_DATA_TIMED field names (table), 2-29
- NCTYPE_CAN_FRAME field names (table), 2-39
- NCTYPE_CAN_FRAME_TIMED field names (table), 2-27
- ncWaitForState function, 2-36
 - description, 2-36
 - examples, 2-37
 - format, 2-36
 - input, 2-36
 - output, 2-36
 - purpose, 2-36
 - return status, 2-37
- ncWrite function, 2-38
 - CAN Network Interface Object, 2-39
 - NCTYPE_CAN_FRAME field names (table), 2-39
 - CAN Object, 2-40
 - NCTYPE_CAN_DATA field names (table), 2-40
 - description, 2-38
 - examples, 2-41
 - format, 2-38
 - input, 2-38
 - purpose, 2-38
 - return status, 2-40
- NI Developer Zone, C-1
- NI-CAN functions, 2-1
 - CAN Network Interface Object, 2-1
 - CAN Object, 2-1
 - description, 2-1
 - examples, 2-2
 - format, 2-1
 - function names, 2-1
 - input and output, 2-1
 - list (table), 2-2
 - ncAction, 2-3
 - ncCloseObject, 2-6
 - ncConfig, 2-7
 - ncCreateNotification, 2-12
 - ncCreateOccurrence, 2-17
 - ncGetAttribute, 2-20

- ncOpenObject, 2-22
- ncRead, 2-25
- ncReadMult, 2-30
- ncReset, 2-33
- ncSetAttribute, 2-34
- ncWaitForState, 2-36
- ncWrite, 2-38
- purpose, 2-1
- return status, 2-1
- NI-CAN host data types, 1-1
 - data types (table), 1-1
- NI-CAN object states, A-1
 - state format (figure), A-1
 - states (table), A-1
- NI-CAN objects, 3-1
 - attributes, 3-1
 - CAN Network Interface Object, 3-2
 - CAN Object, 3-17
 - description, 3-1
 - encapsulates, 3-1
 - object names, 3-1
- NI-CAN status codes and qualifiers, B-4
 - summary of status codes (table), B-4
- NI-CAN status format, B-1
 - checking status in C, B-3
 - checking status in LabVIEW, B-2
 - code, B-2
 - error/warning indicators (severity), B-1
 - determining severity of status (table), B-2
 - format (figure), B-1
 - qualifier, B-2

Q

qualifiers. *See* status codes and qualifiers.

R

- Receive Periodically Using Remote (NC_CAN_COMM_RX_PERIODIC), 3-28
- Receive Unsolicited (NC_CAN_COMM_RX_UN SOL), 3-28
- Receive Value by Call Using Remote (NC_CAN_COMM_RX_BY_CALL), 3-29
- related documentation, *xii*
- RTSI programming, 4-1
 - attributes, 4-2
 - NC_ATTR_RT SI_FRAME, 4-5
 - NC_ATTR_RT SI_MODE, 4-2
 - NC_ATTR_RT SI_SIG_BEHAV, 4-4
 - NC_ATTR_RT SI_SIGNAL (RTSI Line Number), 4-4
 - NC_ATTR_RT SI_SKIP, 4-5
 - description, 4-1
 - examples, 4-5

S

- status codes and qualifiers, B-1
 - checking status
 - in C/C++, B-3
 - in LabVIEW, B-2
 - NC_ERR_ALREADY_OPEN (0006 Hex), B-9
 - NC_ERR_BAD_NAME (0003 Hex), B-7
 - NC_ERR_BAD_PARAM (0004 Hex), B-7
 - NC_ERR_BAD_VALUE (0005 Hex), B-8
 - NC_ERR_CAN_BUS_OFF (0101 Hex), B-11
 - NC_ERR_DRIVER (0002 Hex), B-6
 - NC_ERR_NOT_STOPPED (0007 Hex), B-9
 - NC_ERR_OLD_DATA (0009 Hex), B-11

NC_ERR_OVERFLOW (0008 Hex), B-9
 NC_ERR_TIMEOUT (0001 Hex), B-5
 NC_SUCCESS (0000 Hex), B-5
 summary of status codes (table), B-4
 summary of status codes (table), B-4
 system integration, by National
 Instruments, C-1

T

technical support resources, C-1
 Transmit Data by Call
 (NC_CAN_COMM_TX_BY_CALL), 3-30
 Transmit Data Periodically
 (NC_CAN_COMM_TX_
 PERIODIC), 3-29

Transmit Periodic Waveform
 (NC_CAN_COMM_TX_
 WAVEFORM), 3-31
 Transmit Value by Response Only
 (NC_CAN_COMM_TX_RESP_
 ONLY), 3-30

U

using this manual set, *xi*

W

Web support from National Instruments, C-1
 worldwide technical support, C-2